



Citrix ADC SDX

Contents

Citrix ADC SDX hardware-software compatibility matrix	3
SDX hardware platforms	6
Citrix ADC SDX 8015, SDX 8400, and SDX 8600	6
Citrix ADC SDX 8900	8
Citrix ADC SDX 11500, SDX 13500, SDX 14500, SDX 16500, SDX 18500, and SDX 20500	10
Citrix ADC SDX 11515, SDX 11520, SDX 11530, SDX 11540, and SDX 11542	12
Citrix ADC SDX 14000	14
Citrix ADC SDX 14000-40G	17
Citrix ADC SDX 14xxx-40S	18
Citrix ADC SDX 14030 FIPS, 14060 FIPS, 14080 FIPS	20
Citrix ADC SDX 15000	22
Citrix ADC SDX 15000-50G	24
Citrix ADC SDX 17500, SDX 19500, and SDX 21500	26
Citrix ADC SDX 17550, SDX 19550, SDX 20550, and SDX 21550	28
Citrix ADC SDX 22040, SDX 22060, SDX 22080, SDX 22100, and SDX 22120	30
Citrix ADC SDX 24100 and SDX 24150	33
Citrix ADC SDX 25100A, SDX 25160A	35
Citrix ADC SDX 25100-40G	36
Citrix ADC SDX 26000	39
Citrix ADC SDX 26000-50S	41
Citrix ADC SDX 26000-100G	43
Common hardware components	46
Field replaceable units	57

Safety, cautions, warnings, and other information	63
Prepare for installation	64
Install the hardware	66
Initial configuration	76
Lights out management port of the Citrix ADC SDX appliance	81
Configure the network settings on the LOM port	83
Installing a certificate and key on the LOM GUI	88
Obtaining the MAC address, serial number, and host properties of the appliance	94
Perform power control operations by using the LOM port	95
Restoring the BMC configuration to factory defaults	97
Specifying the port for IPMI BMC failover	98
Using the BIOS POST code to detect errors	98
Hardware health attributes of Citrix ADC SDX appliances	99
Fortville NIC firmware upgrade on Citrix ADC SDX appliances	108
Converting a Citrix ADC MPX appliance to a Citrix ADC SDX appliance	109
Converting a Citrix ADC MPX 11515/11520/11530/11540/11542 appliance to a Citrix ADC SDX 11515/11520/11530/11540/11542 appliance	110
Converting a Citrix ADC MPX 8005/8010/8015/8200/8400/8600/8800 appliance to a Citrix ADC SDX 8010/8015/8400/8600 appliance	119
Converting a Citrix ADC MPX 24100 and 24150 appliance to a Citrix ADC SDX 24100 and 24150 appliance	123
Convert a Citrix ADC MPX 14020/14030/14040/ 14060/14080/14100 appliance to a Citrix ADC SDX 14020/14030/14040/ 14060/14080/14100 appliance	126
Convert a Citrix ADC MPX 14020 40G, MPX 14040 40G, MPX 14060 40G, MPX 14080 40G appliance to a Citrix ADC SDX 14020 40G, SDX 14040 40G, SDX 14060 40G, SDX 14080 40G appliance	133

Convert a Citrix ADC MPX 8900 appliance to a Citrix ADC SDX 8900 appliance	153
Convert a Citrix ADC MPX 15000 appliance to a Citrix ADC SDX 15000 appliance	162
Troubleshooting	181

Citrix ADC SDX hardware-software compatibility matrix

October 11, 2021

Keep the following points in mind about Citrix ADC SDX hardware-software and feature-software compatibility:

- For each platform, only the starting build for each release is mentioned. All subsequent builds within a release are supported.
- In 10.5 and prior releases, the SDX appliance was shipped with a virtual bundle. The bundle included a specific combination of Management Service image, Citrix Hypervisor image, Citrix Hypervisor supplemental packs.
- From 11.0 and later releases, the single bundle image is shipped, which combines all the components.
- Any combinations of SDX image version and VPX image versions are supported as long as they meet minimum version requirements for a particular hardware platform.
- From 12.0 57.19, the single bundle image also includes the lights-out management (LOM) firmware.
- Direct upgrade from version 10.5 to version 13.1 is not supported. First upgrade from 10.5 to 11.1 or 12.0 or 12.1, and then upgrade to SDX 13.1.
- Usually, the SDX image and the VPX image are not interdependent, which means the SDX appliance and the VPX instances need not have the same image version.

Exception: If you provision a new VPX instance or upgrade an existing VPX instance to 12.0-58.15, you must also upgrade the SDX version to 12.0-58.15. See <https://support.citrix.com/article/CTX236730>.

If you use Citrix ADM to manage Citrix ADC appliances running 12.0–58.15, you must upgrade Citrix ADM to 12.0-58.15.

The following tables list the compatibility matrix for all Citrix ADC SDX hardware platforms and the SDX and VPX images supported on these platforms.

How to read the table

The SDX image version and the VPX image version are listed for each platform. The SDX image and the VPX image are not interdependent, which means the SDX appliance and the VPX instances need not have the same image version. Check the note for exception to compatibility. The starting builds are listed.

Hardware platforms/SDX SBI version and VPX image version	11.1	12.1	13.0	13.1
SDX 8015	11.1-47.14	12.1-48.13	13.0-36.x	13.1-4.x
SDX 8400/8600	11.1-47.14	12.1-48.13	13.0-36.x	13.1-4.x
SDX 8920/8930	11.1-57.11 (See note after the table)	12.1-48.13	13.0-36.x	13.1-4.x
SDX 11500/13500/14500/16500/18500/20500	11.1-47.14	12.1-48.13	13.0-36.x	13.1-4.x
SDX 11515/11520/1153	11.1-47.14	12.1-48.13	13.0-36.x	13.1-4.x
SDX 14020/14030/14040/14060/14080/14100	11.1-47.14	12.1-48.13	13.0-36.x	13.1-4.x
SDX 14020- 40G/14040- 40G/14060- 40G/14080- 40G/14100-40G	11.1-47.14	12.1-48.13	13.0-36.x	13.1-4.x
SDX 14040- 40S/14060- 40S/14080- 40S/14100-40S	11.1-48.10	12.1-48.13	13.0-36.x	13.1-4.x
SDX 14030 FIPS/14060 FIPS/14080 FIPS	11.1-52.13	12.1-48.13	13.0-36.x	13.1-4.x
SDX 15020/15030/15040/15060/15080/15100/15120	11.1-63.x	12.1-56.x	13.0-52.x	13.1-4.x

Hardware platforms/SDX SBI version and VPX image version	11.1	12.1	13.0	13.1
SDX 15020-50G/15030-50G/15040-50G/15060-50G/15080-50G/15100-50G/15120-50G	11.1-59.10	12.1-48.13	13.0-36.x	13.1-4.x
SDX 22040/22060/22080/22100/22120	11.1-47.14	12.1-48.13	13.0-36.x	13.1-4.x
SDX 24100/24150	11.1-47.14	12.1-48.13	13.0-36.x	13.1-4.x
SDX 25100A/25160A/25200A	11.1-51.21	12.1-48.13	13.0-36.x	13.1-4.x
SDX 25100-40G/25160-40G/25200-40G	11.1-51.21	12.1-48.13	13.0-36.x	13.1-4.x
SDX 26100/26160/26200	11.1-63.9	12.1-56.x	13.0-52.x	13.1-4.x
SDX 26100-100G/26160-100G/26200-100G	11.1-58.13	12.1-48.13	13.0-36.x	13.1-4.x
SDX 26100-50S/26160-50S/26200-50S	11.1-63.9	12.1-56.x	13.0-52.x	13.1-4.x

Notes:

- On the Citrix ADC SDX 8900 appliance, the 11.1 56.15 VPX image is supported. SDX 11.1 56.15 image is not supported.
- Citrix ADC Secure Web Gateway (SWG) is supported from release 12.0 56.20 and later.
- Citrix ADC cluster is not supported on Citrix SDX SWG instances.

Related information

For information about how to upgrade the Citrix ADC SDX appliance and the VPX instance, see the following topics.

- [Single bundle upgrade for 12.1 release](#)
- [Demystifying the Citrix ADC SDX appliance upgrade process](#)

SDX hardware platforms

June 24, 2021

The various Citrix ADC hardware platforms offer a wide range of features, communication ports, and processing capacities. All platforms have multicore processors.

The Citrix ADC SDX appliance is a multitenant platform on which you can provision and manage multiple virtual instances. All Citrix ADC appliances have front to rear airflow.

Citrix ADC SDX 8015, SDX 8400, and SDX 8600


August 18, 2020

The Citrix ADC SDX 8015, SDX 8400, and SDX 8600 are 1U appliances. Each model has one quad-core processor (8 cores with hyper-threading) and 32 GB of memory. The SDX 8015/8400/8600 appliances are available in two port configurations:

- Six 10/100/1000Base-T copper Ethernet ports and six 1G SFP ports (6x10/100/1000Base-T copper Ethernet ports + 6x1G SFP)
- Six 10/100/1000Base-T copper Ethernet ports and two 10G SFP+ ports (6x10/100/1000Base-T copper Ethernet ports + 2x10G SFP+)


The following figure shows the front panel of the SDX 8015/8400/8600 (6x10/100/1000Base-T copper Ethernet ports + 6x1G SFP) appliance.

Figure 1. Citrix ADC SDX 8015/8400/8600 (6x10/100/1000Base-T copper Ethernet ports + 6x1G SFP), front panel

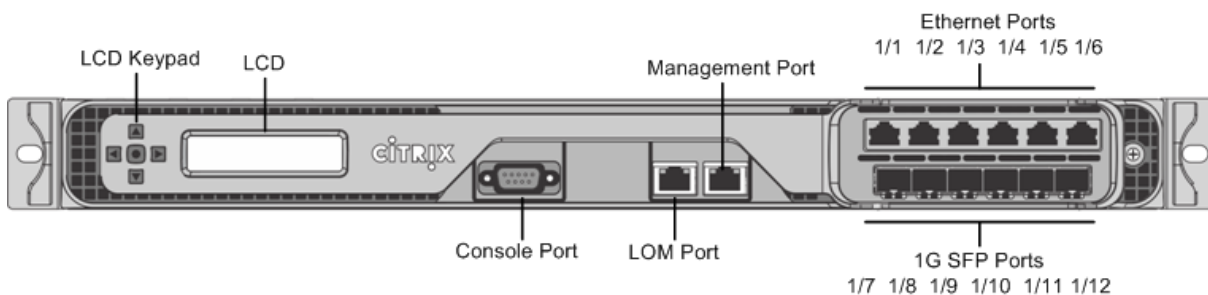

The following figure shows the front panel of the SDX 8015/8400/8600 (6x10/100/1000Base-T copper Ethernet ports + 2x10G SFP+) appliance.

Figure 2. Citrix ADC SDX 8015/8400/8600 (6x10/100/1000Base-T copper Ethernet ports + 2x10G SFP+), front panel

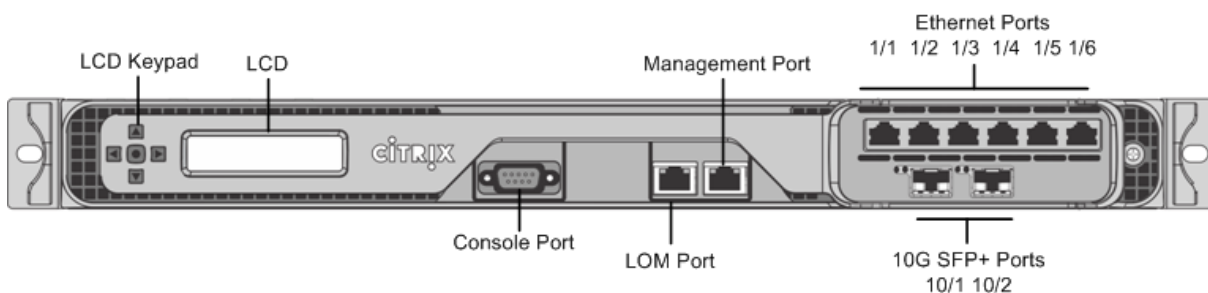


Depending on the model, the appliance has the following ports:

- RS232 serial console port.
- One 10/100Base-T copper Ethernet Port (RJ45), also called LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- One 10/100/1000Base-T copper Ethernet management port (RJ45), numbered 0/1. The management port is used to connect directly to the appliance for system administration functions.
- Network Ports
 - SDX 8015/8400/8600 (6x10/100/1000Base-T copper Ethernet ports + 6x1G SFP). Six 10/100/1000BASE-T copper Ethernet ports (RJ45) numbered 1/1, 1/2, 1/3, 1/4, 1/5, and 1/6 on the top row from left to right. Six 1-gigabit copper or fiber 1G SFP ports numbered 1/7, 1/8, 1/9, 1/10, 1/11, and 1/12 on the bottom row from left to right.
 - SDX 8015/8400/8600 (6x10/100/1000Base-T copper Ethernet ports + 2x10G SFP+). Six 10/100/1000BASE-T copper Ethernet ports (RJ45) numbered 1/1, 1/2, 1/3, 1/4, 1/5, and 1/6 on the top row from left to right and two 10-gigabit SFP+ ports numbered 10/1 and 10/2 on the bottom row from left to right.

The following figure shows the back panel of the SDX 8015/8400/8600 appliance.

Figure 3. Citrix ADC SDX 8015/8400/8600 appliance, back panel

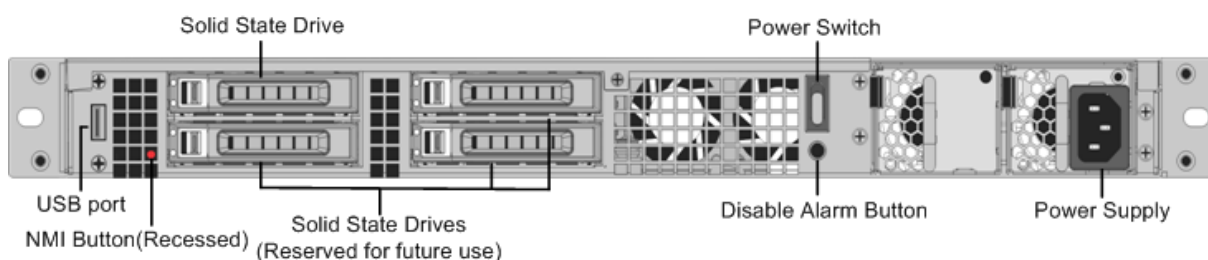

The following components are visible on the back panel of the SDX 8015/8400/8600 appliance:

- One 300 GB or larger removable solid-state drive, which is used to store the Citrix ADC software and user data.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

- Power switch, which turns off power to the appliance, as if you were to unplug the power supply. Press the switch for five seconds to shut off the power.
- USB port (reserved for a future release).
- Non-maskable interrupt (NMI) button, which is used at the request of Technical Support to produce a Citrix ADC core dump. Use a pen, pencil, or other pointed object to press this red button, which is recessed to prevent unintentional activation.
- **Disable alarm button**, which is nonfunctional. This button is functional only if you install a second power supply.

Press this button to stop the power alarm from sounding when either of the following conditions is true:

- You have plugged the appliance into only one power outlet.
 - One power supply is malfunctioning, and you want to continue operating the appliance until it is repaired.
- Single power supply, rated at 450 watts, 110–220 volts.

Citrix ADC SDX 8900

August 18, 2020

The Citrix ADC SDX 8900 appliance is a 1U appliance. This platform has a single 8-core processor and 32 GB of memory. The appliance provides a total of 10 network ports:

- Six 10/100/1000Base-T RJ45 copper Ethernet Ports.
- Four 10G SFP+ Ethernet Ports.


1G copper transceivers are supported in 10G slots. 1G fiber transceivers are not supported.

The appliance comes with two VPX instances and supports up to seven instances. You can separately buy extra five instances.

For information on the software releases supported on the Citrix ADC hardware platforms, see [Citrix ADC SDX Hardware-Software Compatibility Matrix](#).

The figures are for illustrative purposes only.


Figure 1. Citrix ADC SDX 8900 front panel

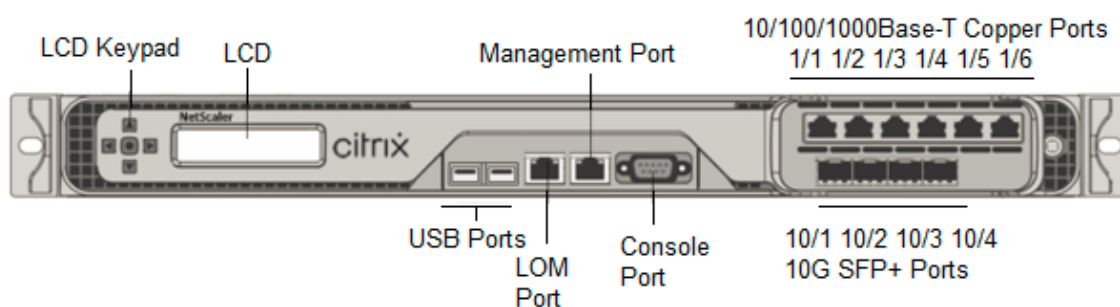

The Citrix ADC SDX 8900 appliances have the following ports:

- RS232 serial Console Port.
- One 10/100/1000Base-T RJ45 copper Ethernet LOM Port. Use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- One 10/100/1000Base-T RJ45 copper Ethernet Management Port, numbered 0/1. This port is used to connect directly to the appliance for Citrix ADC administration functions.
- Six 10/100/1000Base-T RJ45 copper Ethernet Ports, numbered 1/1 to 1/6 from left to right.
- Four 10G SFP+ Ethernet Ports, numbered 10/1 to 10/4 from left to right.
- USB port (reserved for a future release).

Figure 2. Citrix ADC SDX 8900 back panel

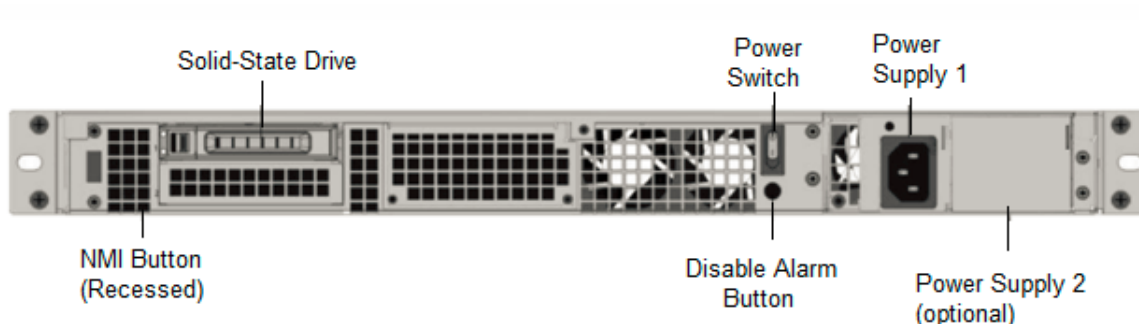

The following components are visible on the back panel of the SDX 8900 appliances:

- One 240 GB or larger removable solid-state drive (SSD).

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

- Power switch, which turns power to the appliance on or off.
 - If the OS is functional, press the switch for less than two seconds to power down the system with a graceful shutdown.
 - If the OS is not responsive, press the power switch for more than 4 seconds to force the power off.
- One power supply, 100–240 VAC (second power supply for redundancy is a customer installable option). Each power supply has an LED indicating its status:

LED color	LED indicates
OFF	No power to any power supply in the appliance.
Flashing RED	No power to this power supply.
Flashing GREEN	Power supply is in standby mode.
GREEN	Power supply is functional.
RED	Power supply failure.

- **Disable alarm button**, which is functional only when the appliance has two power supplies. Press this button to silence the power alarm when one of two power supplies loses input power (second power supply optional) or when a power supply is malfunctioning.
- Non-Maskable Interrupt (NMI) Button, used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The **NMI** Button is also available remotely over the network in the LOM GUI, in the **Remote Control** menu. For more information, see [Lights out management port of the Citrix ADC SDX appliance](#).

Citrix ADC SDX 11500, SDX 13500, SDX 14500, SDX 16500, SDX 18500, and SDX 20500

January 11, 2021


Note: This platform has reached its end of life.

The Citrix ADC models SDX 11500/13500/14500/16500/18500/20500 are 2U appliances. Each model has two 6-core processors for a total of 12 physical cores (24 cores with hyper-threading), and 48 GB

of memory.

The following figure shows the front panel of the SDX 11500/13500/14500/16500/18500/20500 appliance.

Figure 1. Citrix ADC SDX 11500/13500/14500/16500/18500/20500 appliance, front panel

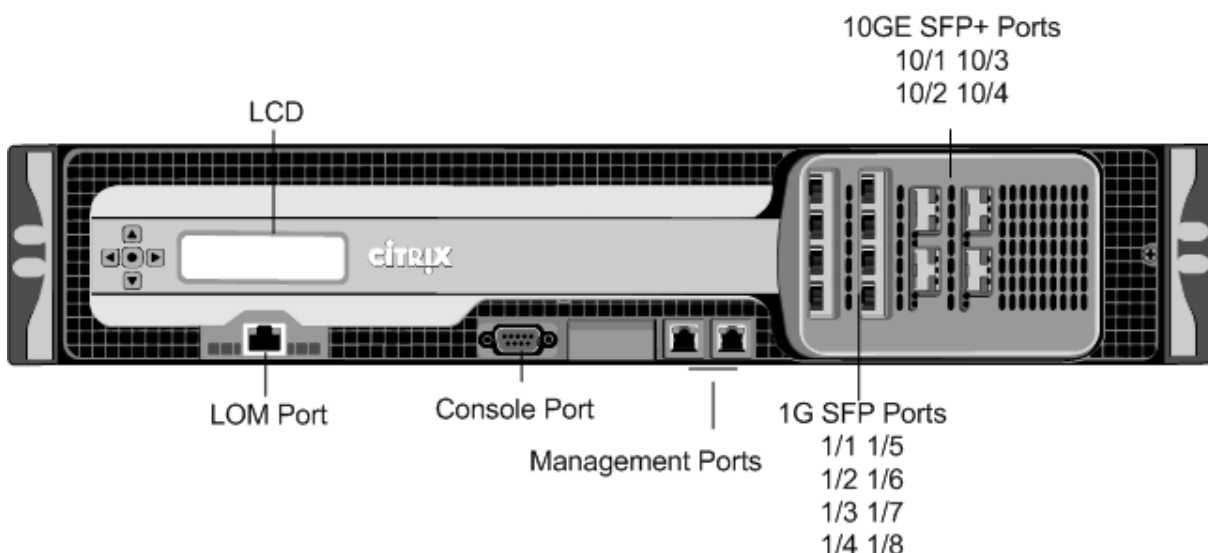


The SDX 11500/13500/14500/16500/18500/20500 appliances have the following ports:

- 10/100Base-T copper Ethernet Port (RJ45), also called LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
Note: The LEDs on the LOM port are not operational by design.
- RS232 serial console port.
- Two 10/100/1000Base-T copper Ethernet management ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Eight 1G SFP ports numbered 1/1, 1/2, 1/3, 1/4 from top to bottom in the first column, and 1/5, 1/6, 1/7, and 1/8 from top to bottom in the second column.
- Four 10GE SFP+ ports numbered 10/1 and 10/2 from top to bottom in the first column, and 10/3 and 10/4 from top to bottom in the second column.

The following figure shows the back panel of the SDX 11500/13500/14500/16500/18500/20500 appliance.

Figure 2. Citrix ADC SDX 11500/13500/14500/16500/18500/20500 appliance, back panel

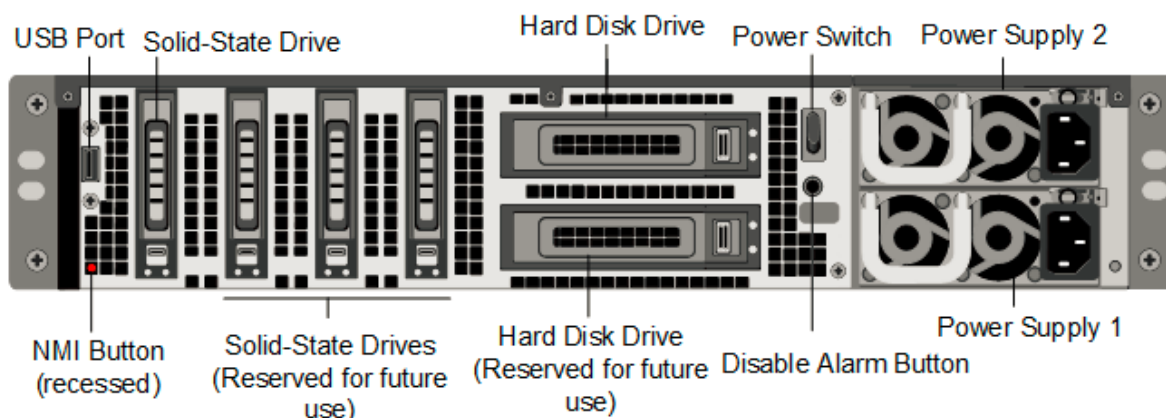

The following components are visible on the back panel of the SDX 11500/13500/14500/16500/18500/20500 appliance:

- One 160 GB or larger removable solid-state drive that is used to store the Citrix ADC software.
Note: Drive densities might increase as components become EOL but its size is never smaller than the original.
- USB port (reserved for a future release).
- Power switch, which turns off power to the appliance, as if you were to unplug the power supply. Press the switch for five seconds to shut off the power.
- Non-maskable interrupt (NMI) Button that is used at the request of Technical Support and produces a core dump on the Citrix ADC appliance. Use a pen, pencil, or other pointed object to press this red button, which is recessed to prevent unintentional activation.
- Two removable hard-disk drives that are used to store user data.
- **Disable alarm button.** This button is functional only when the appliance has two power supplies.

Press this button to stop the power alarm from sounding when either of the following conditions is true:

- You have plugged the appliance into only one power outlet.
 - One power supply is malfunctioning, and you want to continue operating the appliance until it is repaired.
- Dual power supplies, each rated at 650 watts, 110–220 volts.

Citrix ADC SDX 11515, SDX 11520, SDX 11530, SDX 11540, and SDX 11542


August 18, 2020

The Citrix ADC models

SDX 11515/11520/11530/11540/11542 are 2U appliances. Each model has two 6-core processors for a total of 12 physical cores (24 cores with hyper-threading), and 48 GB of memory.

The following figure shows the front panel of the SDX 11515/11520/11530/11540/11542 appliance.

Figure 1. Citrix ADC SDX 11515/11520/11530/11540/11542 appliance, front panel

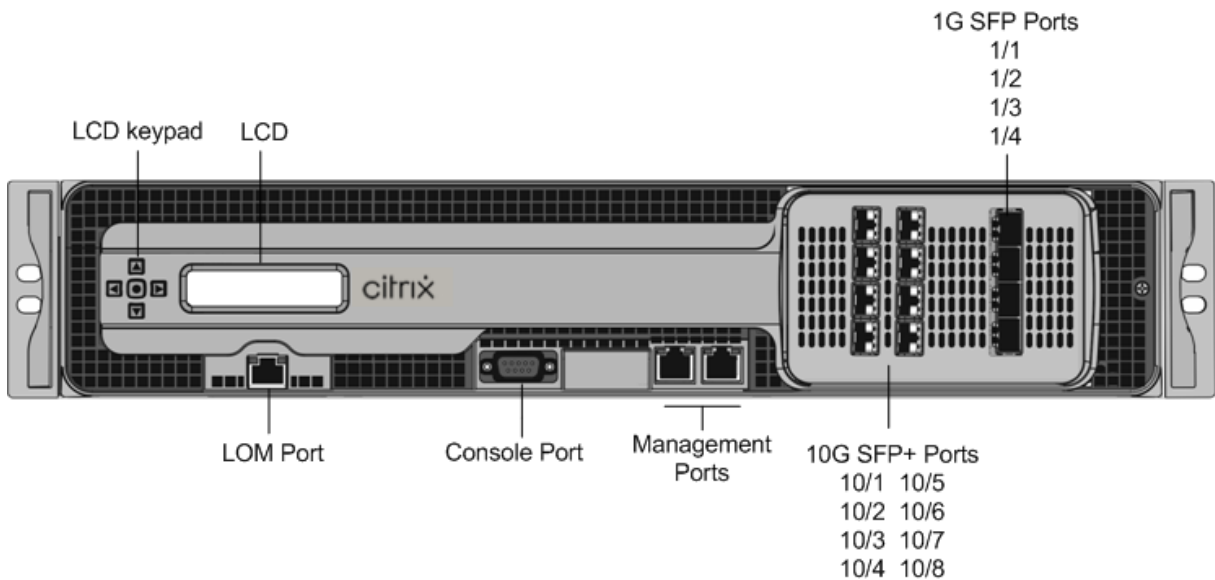


The SDX 11515/11520/11530/11540/11542 appliances have the following ports:

- RS232 serial console port.
- 10/100Base-T copper Ethernet Port (RJ45), also called LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
Note: The LEDs on the LOM port are not operational by design.
- Two 10/100/1000Base-T copper Ethernet management ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Eight 10G SFP+ ports and four copper or fiber 1G SFP ports.

The following figure shows the back panel of the SDX 11515/11520/11530/11540/11542 appliance.

Figure 2. Citrix ADC SDX11515/11520/11530/11540/11542 appliance, back panel

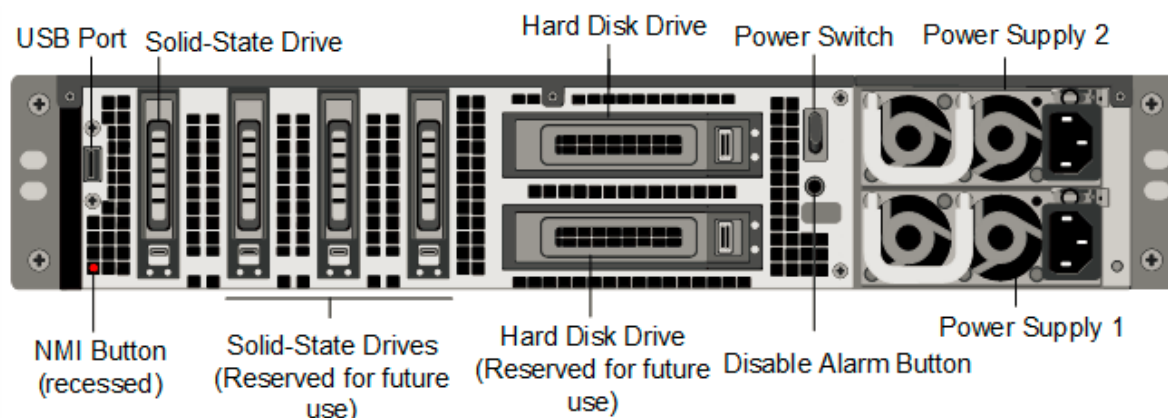

The following components are visible on the back panel of the SDX 11515/11520/11530/11540/11542 appliance:

- One 256 GB or larger removable solid-state drive that is used to store the Citrix ADC software.
Note: Drive densities might increase as components become EOL but its size is never smaller than the original.
- USB port (reserved for a future release).
- Power switch, which turns off power to the appliance, as if you were to unplug the power supply. Press the switch for five seconds to shut off the power.
- Non-maskable interrupt (NMI) Button that is used at the request of Technical Support and produces a core dump on the Citrix ADC appliance. Use a pen, pencil, or other pointed object to press this red button, which is recessed to prevent unintentional activation.
- Two removable hard-disk drives that are used to store user data.
- **Disable alarm button.** This button is functional only when the appliance has two power supplies.

Press this button to stop the power alarm from sounding when either of the following conditions is true:

- You have plugged the appliance into only one power outlet.
 - One power supply is malfunctioning, and you want to continue operating the appliance until it is repaired.
- Dual power supplies, each rated at 650 watts, 110–220 volts.

Citrix ADC SDX 14000

August 29, 2020


The Citrix ADC SDX 14020/14030/14040/14060/14080/14100 are 2U appliances. Each model has two 6-core processors and 64 GB of memory and sixteen 10G SFP+ ports (16x10G SFP+).

Note

For information about Citrix ADC SDX hardware and component compatibility matrix, see [Citrix ADC SDX Hardware-Software Compatibility Matrix](#).

The following figure shows the front panel of the SDX 14020/14030/14040/14060/14080/ 14100 (16x10G SFP+) appliance.

Figure 1. Citrix ADC SDX 14020/14030/14040/14060/14080/14100 (16x10G SFP+), front panel

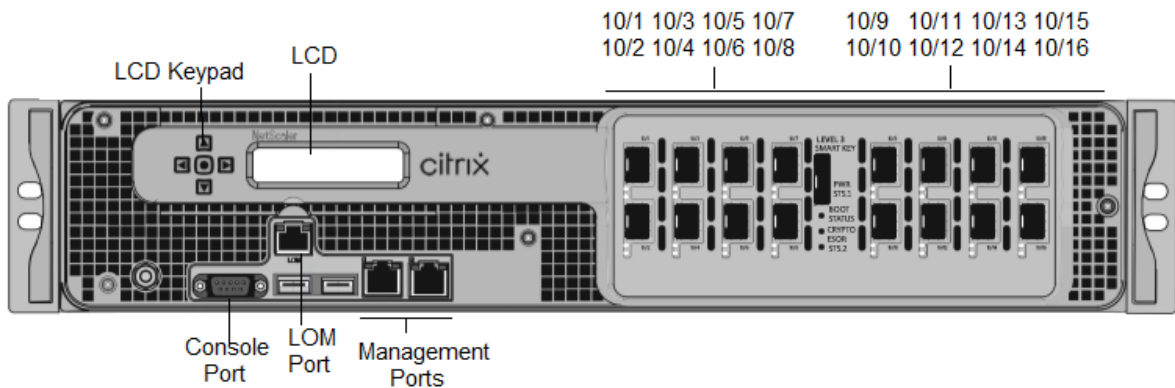

The Citrix ADC SDX 14020/14030/14040/14060/14080/14100 appliances have the following ports:


- RS232 serial Console Port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T copper Ethernet management ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Network ports, sixteen 10G SFP+ ports (16x10G SFP+).
- USB ports (reserved for a future release).

Note

The 10G SFP+ ports on these appliances support copper 1G SFP transceivers.

The following figure shows the back panel of the SDX 14020/14030/14040/14060/14080/ 14100 appliance.

Figure 2. Citrix ADC SDX 14020/14030/14040/14060/14080/14100, back panel

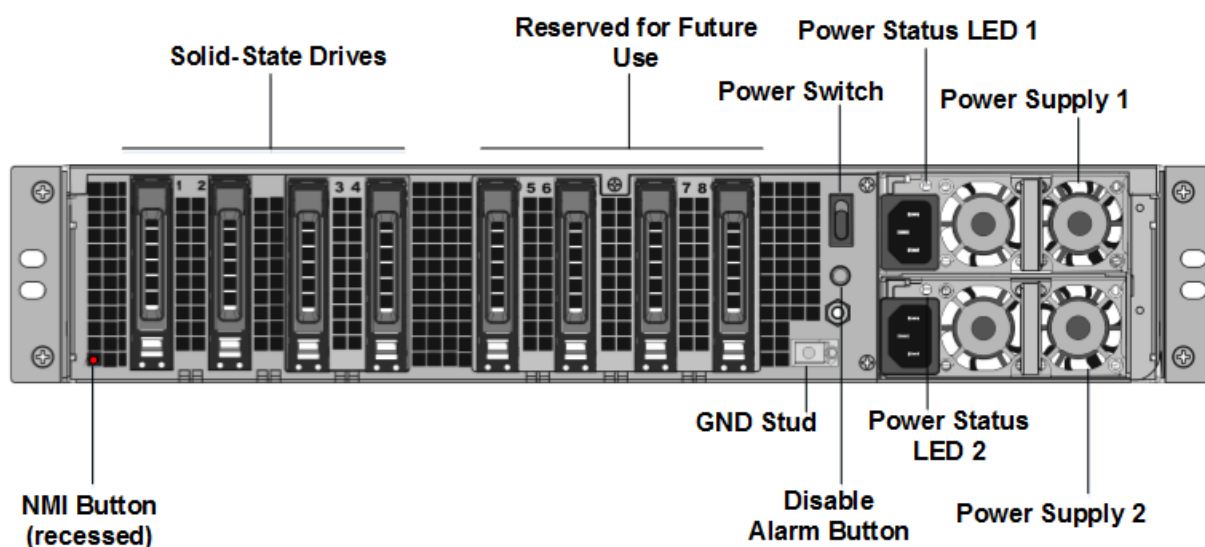

The following components are visible on the back panel of the SDX 14020/14030/14040/14060/14080/14100 appliance:

- Two 240 GB or larger removable solid-state drives in a redundant array of independent disks (RAID) configuration.

Note: These drives store the Citrix software, and cannot be increased by users.

- Two to six 300 GB or larger solid-state drives.

Note: These drives are used to provision VPX instances. Contact Citrix Sales Support to purchase extra drives.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

For more information about managing RAID allocation, see [Managing RAID disk allocation on SDX 22XXX](#).

- **Power switch** which turns power to the appliance on or off. Press the switch for less than two seconds to shut off the power.
- **Two power supplies.** each rated at 1000 watts, 100–240 volts. Each power supply has an LED that indicates the status of the power supply, as described in [Common hardware components](#).
- ****Disable alarm button.**** which is functional only when the appliance has two power supplies. Press this button to stop the power alarm from sounding when either of the following conditions is true:
 - You have plugged the appliance into only one power outlet
 - One power supply is malfunctioning and you want to continue operating the appliance until it is repaired.

- **Non-maskable interrupt (NMI) Button.** used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information about the lights out management port of the appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

Note: If you buy an instance license pack for SDX 14000 that includes extra SSDs, read [CTX215581](#). Complete the steps for adding a logical drive before trying to use the additional instance licenses.

Citrix ADC SDX 14000-40G

August 19, 2020

The Citrix NetScaler SDX 14020-40G, SDX 14040-40G, SDX 14060-40G, SDX 14080-40G, and SDX 14100-40G are 2U appliances. Each model has two 6-core processors and 64 GB of memory. The SDX 14020-40G/14040-40G/14060-40G/14080-40G/14100-40G appliances are available in the four-40G QSFP+ ports and sixteen 10G SFP+ ports (4x40G QSFP+ + 16x10G SFP+) configuration.

For information on the software releases supported on the Citrix ADC hardware platforms, see [Citrix ADC SDX hardware-software compatibility matrix](#).

The following figure shows the front panel of the SDX 14000-40G appliance.

Figure 1. Citrix NetScaler SDX 14020-40G, SDX 14040-40G, SDX 14060-40G, SDX 14080-40G, SDX 14100-40G (4x40G QSFP+ + 16x10G SFP+), front panel

The Citrix ADC SDX 14000-40G appliances have the following ports:

- RS232 serial Console Port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the NetScaler software.
- Two 10/100/1000Base-T copper Ethernet Management Ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Network Ports: four-40G QSFP+ ports and sixteen 10G SFP+ ports (4x40G QSFP+ + 16x10G SFP+).
- USB ports (reserved for a future release).

The following figure shows the back panel of the SDX 14000-40G appliance.

Figure 2. Citrix ADC SDX 14020/14040/14060/14080/14100-40G (4x40G QSFP+, 16x10G SFP+), back panel

The following components are visible on the back panel of the SDX 14000-40G appliance:

- Two 240 GB or larger removable solid-state drives (SSDs). The two leftmost solid-state drives store the NetScaler software. The next two solid-state drives store user data. The remaining four solid-state drives are reserved for future use. These appliances are a redundant array of independent disks (RAID) devices. In a RAID configuration, the same data is stored on multiple drives to improve performance, increase storage capacity, lower the risk of data loss, and provide fault tolerance.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

- Power switch, which turns the power to the appliance on or off. Press the switch for less than two seconds to shut off the power.
- Two power supplies, each power supply is rated at 1000 watts, 100–240 volts. Each power supply has an LED that indicates the status of the power supply.
- **Disable alarm button.** This button is functional only when the appliance has two power supplies. Press this button to stop the power alarm from sounding when either of the following conditions is true:
 - You have plugged the appliance into only one power outlet.
 - One power supply is malfunctioning and you want to continue operating the appliance until it is repaired.
- Non-maskable interrupt (NMI) button that is used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information about lights out management port of the appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

Citrix ADC SDX 14xxx-40S

August 19, 2020

The Citrix NetScaler SDX 14040-40S, SDX 14060-40S, SDX 14080-40S, and SDX 14100-40S are 2U appliances. Each model has two 6-core processors and 64 GB of memory. The SDX 14040-40S/14060-40S/14080-40S/SDX 14100-40S appliances are available in the four-40S QSFP+ ports and sixteen 10G SFP+ ports (4x40G QSFP+ + 8x10G SFP+) configuration.

For information on the software releases supported on the Citrix ADC hardware platforms, see [Citrix ADC SDX hardware-software compatibility matrix](#).

The following figure shows the front panel of the SDX 14xxx-40S appliance.

Figure 1. Citrix NetScaler SDX 14040-40S, SDX 14060-40S, SDX 14080-40S, SDX 14100-40S (4x40G QSFP+ + 8x10G SFP+), front panel

The Citrix ADC SDX 14xxx-40S appliances have the following ports:

- RS232 serial Console Port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the NetScaler software.
- Two 10/100/1000Base-T copper Ethernet Management Ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Network Ports: four-40S QSFP+ ports and eight 10G SFP+ ports (4x40G QSFP+ + 8x10G SFP+).

The following figure shows the back panel of the SDX 14xxx-40S appliance.

Figure 2. Citrix ADC SDX 14040/14060/14080/14100-40S (4x40G QSFP+, 8x10G SFP+), back panel

The following components are visible on the back panel of the SDX 14xxx-40S appliance:

- Two 240 GB or larger removable solid-state drives (SSDs). The two leftmost solid-state drives store the NetScaler software. The next two solid-state drives store user data. The remaining four solid-state drives are reserved for future use. These appliances are a redundant array of independent disks (RAID) devices. In a RAID configuration, the same data is stored on multiple drives to improve performance, increase storage capacity, lower the risk of data loss, and provide fault tolerance.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

- Power switch, which turns the power to the appliance on or off. Press the switch for less than two seconds to shut off the power.
- Two power supplies, each power supply is rated at 1000 watts, 100–240 volts. Each power supply has an LED that indicates the status of the power supply.
- **Disable alarm button.** This button is functional only when the appliance has two power supplies. Press this button to stop the power alarm from sounding when either of the following conditions is true:
 - You have plugged the appliance into only one power outlet.
 - One power supply is malfunctioning and you want to continue operating the appliance until it is repaired.
- Non-maskable interrupt (NMI) button that is used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information about lights out


management port of the appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

Citrix ADC SDX 14030 FIPS, 14060 FIPS, 14080 FIPS

September 29, 2020

The Citrix ADC models SDX 14030 FIPS, SDX 14060 FIPS, and SDX 14080 FIPS are 2U appliances. Each model has two 6-core processors, 64 GB memory, 16 10G SFP+ ports (16x10G SFP+).

Figure 1. Citrix ADC SDX 14030/14060/14080 FIPS front panel

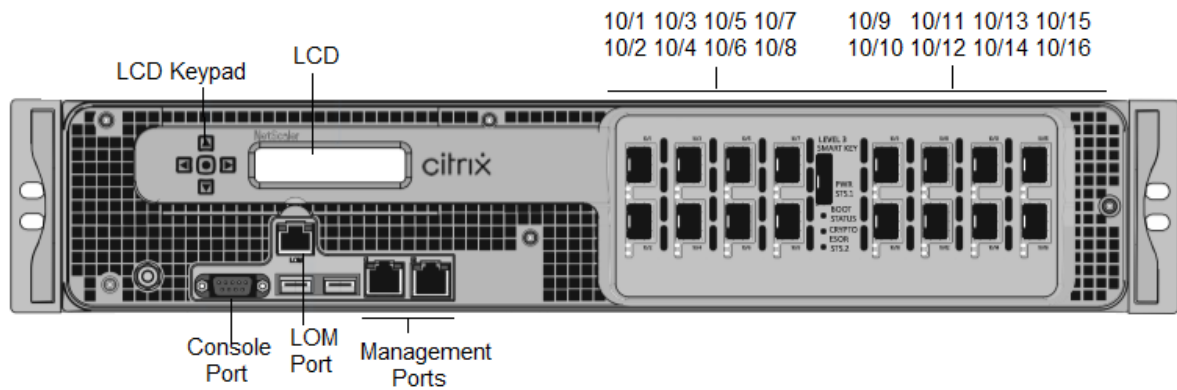


The Citrix ADC SDX 14030/14060/14080 FIPS appliances have the following ports:

- RS232 serial Console Port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T copper Ethernet Management Ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Sixteen 10G SFP+ ports.
- USB ports (reserved for a future release).

Note:

- 10G ports do not support 1G copper or 1G fiber transceivers.
- 40G ports do not support 10G and 1G transceivers.

Figure 2. Citrix ADC SDX 14030/14060/14080 FIPS appliance back panel

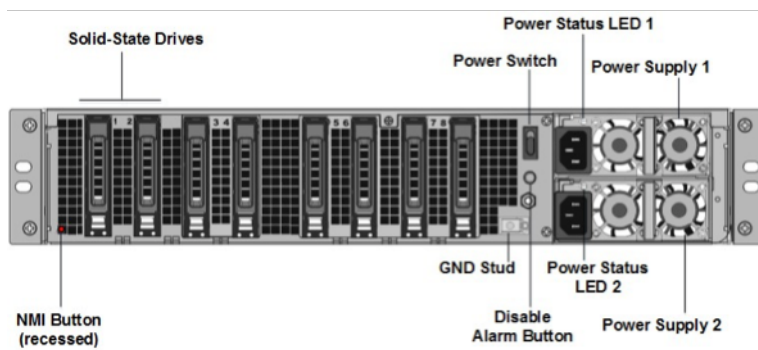

The following components are visible on the back panel of the SDX 14030 FIPS, SDX 14060 FIPS, and SDX 14080 FIPS appliances:

- Two 240 GB or larger removable solid-state drives in a redundant array of independent disks (RAID) configuration.

Note: These drives store the Citrix software, and cannot be increased by users.

- Two to six 300 GB or larger solid-state drives.

Note: These drives are used to provision VPX instances. Contact Citrix Sales Support to purchase extra drives.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

- **Power switch.** Which turns power to the appliance on or off. Press the switch for less than two seconds to shut off the power.
- Two power supplies, each rated at 1000 watts, 100–240 volts. Each power supply has an LED that indicates the status of the power supply, see [Common hardware components](#).
- ****Disable alarm button**.** Which is functional only when the appliance has dual redundant, hot-swappable power supplies. Press this button to silence the power alarm when one of the two power supplies loses input power or when a power supply is malfunctioning.
- **Non-maskable interrupt (NMI) button.** Used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the lights out management GUI, in the Remote Controlment. For more information, see [Lights out management port of the Citrix ADC SDX appliance](#).

See [Configuring an SDX 14000 FIPS appliance](#) for more information about how to configure an SDX 14030/14060/14080 FIPS appliance.

Citrix ADC SDX 15000


August 18, 2020

The Citrix ADC SDX 15020/15030/15040/15060/15080/15100/15120 appliances are 2U appliances. This platform has two 8-core processors and 128 GB of memory. The appliance provides a total of 16 Ethernet 25G ports.

For information on the software releases supported on the Citrix ADC hardware platforms, see [Citrix ADC SDX hardware-software compatibility matrix](#).

The following figure shows the front panel of the SDX 15xxx series appliances.

Figure 1. Citrix ADC SDX 15xxx, front panel

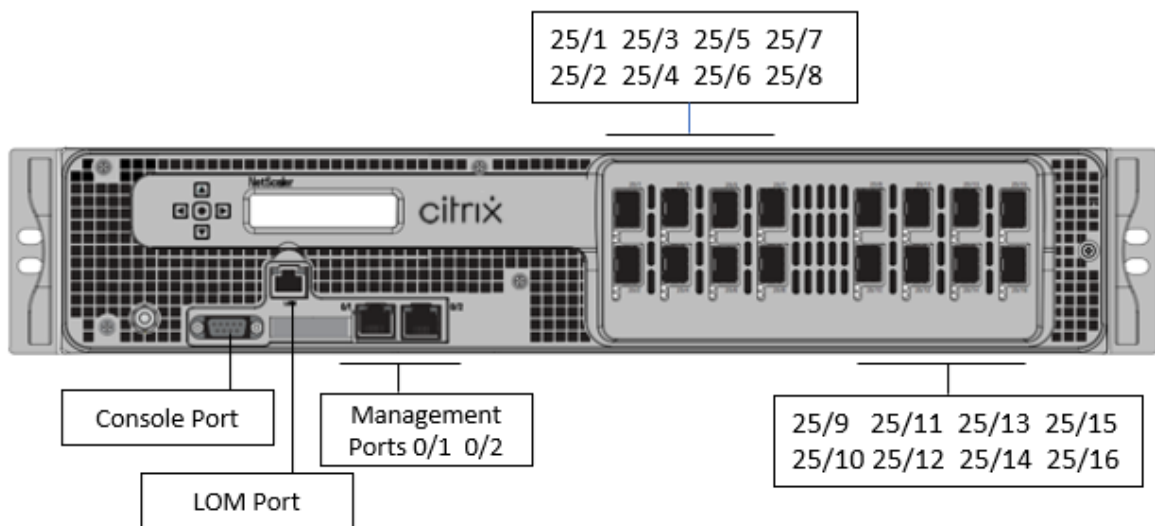


The Citrix ADC SDX 15xxx series appliances have the following ports:

- RS232 serial console port.
- One 10/100/1000Base-T RJ45 copper Ethernet LOM Port. Use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- One 10/100/1000Base-T RJ45 copper Ethernet Management Port, numbered 0/1. This port is used to connect directly to the appliance for Citrix ADC administration functions.
- Sixteen 25G Ethernet ports, numbered 25/1 to 25/16.

The following figure shows the back panel of the SDX 15xxx appliance.

Figure 2. Citrix ADC SDX 15xxx, back panel

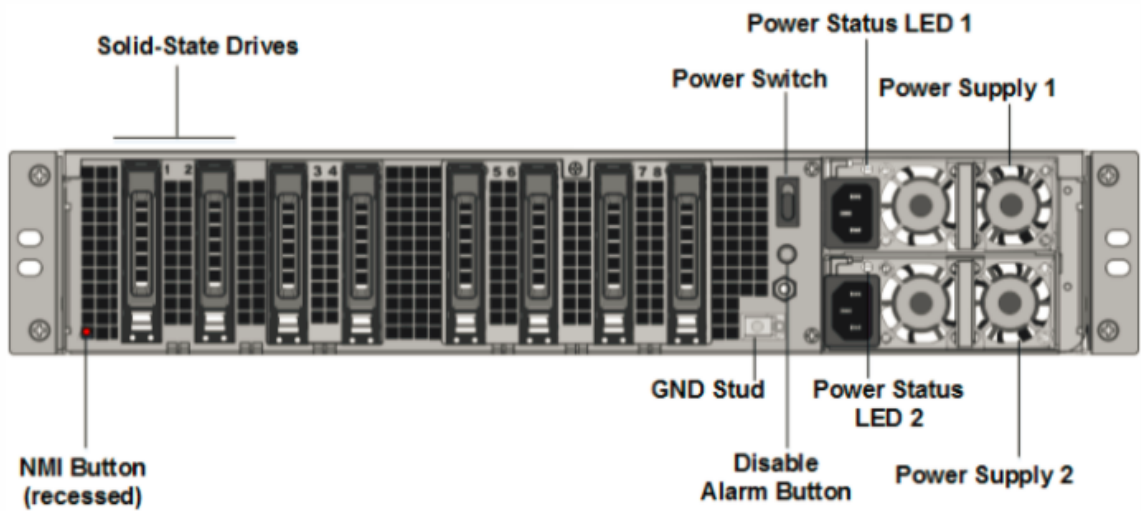

The following components are visible on the back panel of the SDX 15xxx appliance:

- Four 240 GB and two 480 GB removable solid-state drives (SSD).
 - Note:** Drive densities might increase as components become EOL but its size is never smaller than the original.
- Power switch, which turns power to the appliance on or off.
 - If the OS is functional, press the switch for less than two seconds to shut down the system gracefully.
 - If the OS is not responsive, press the power switch for more than 4 seconds to force the power off.
- Two hot-swappable 100–240 VAC input power-supply modules. Each power supply has an LED indicating its status:

LED Color	LED Indicates
OFF	No power to any power supply in the appliance.
Flashing RED	No power to this power supply.
Flashing GREEN	Power supply is in standby mode.
GREEN	Power supply is functional.
RED	Power supply failure.
Flashing RED and GREEN	Warning (OVP/UVP/OCP/OTP/Fan); OVP = Over Voltage Protection; UVP = Under Voltage Protection; OCP = Over Current Protection; OTP = Over Temperature Protection

- **Disable alarm button:** functional only when the appliance has two power supplies. Press this button to silence the power alarm when one of two power supplies loses input power (second power supply optional) or when a power supply is malfunctioning.
- **Non-Maskable Interrupt (NMI) button:** recessed to prevent unintentional activation and used at the request of Technical Support to initiate a core dump. To press this red button, use a pen, pencil, or other pointed object. The NMI button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information, see [Lights out management port of the Citrix ADC SDX appliance](#) topic.

Citrix ADC SDX 15000-50G

August 29, 2020


The Citrix ADC SDX 15020/15030/15040/15060/15080/15100/15120 50G models are 2U appliances. This platform has a dual 8-core processor and 128 GB memory. The SDX 15000-50G appliance provides a total of 12 network ports:

- Eight 10G SFP+ Ethernet Ports
- Four 50G Ethernet Ports

For information about the software releases supported on the Citrix ADC hardware platforms, see [Citrix ADC SDX Hardware and Component Compatibility Matrix](#)

The illustrations in this guide are only indicative and might not represent the actual Citrix ADC appliance.


Figure 1. Citrix ADC SDX 15000-50G, front panel

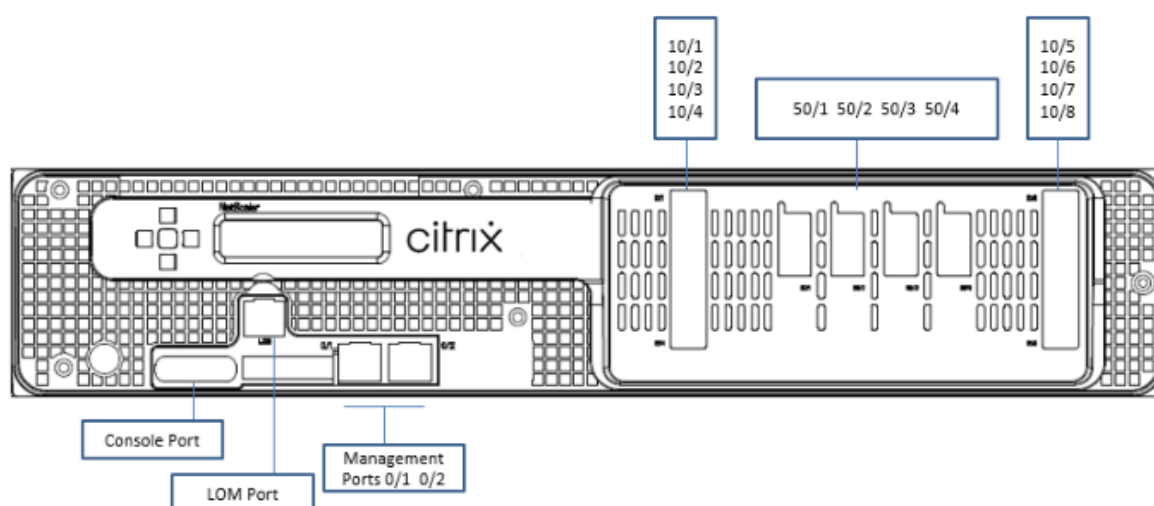

The Citrix ADC SDX 15000-50G appliance has the following ports:

- One RS232 Serial Console Port.
- One 10/100/1000 Base-T RJ45 copper Ethernet lights out management port. Use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T RJ45 copper Ethernet Management Ports, numbered 0/1 and 0/2. These ports are used to connect directly to the appliance for Citrix ADC administration functions.
- Eight 10G SFP+ Ethernet ports, numbered 10/1 to 10/8. Each port has its own LED.
- Four 50G ports, numbered 50/1 to 50/4. Each port has its own LED.

Figure 2. Citrix ADC SDX 15000-50G, rear panel

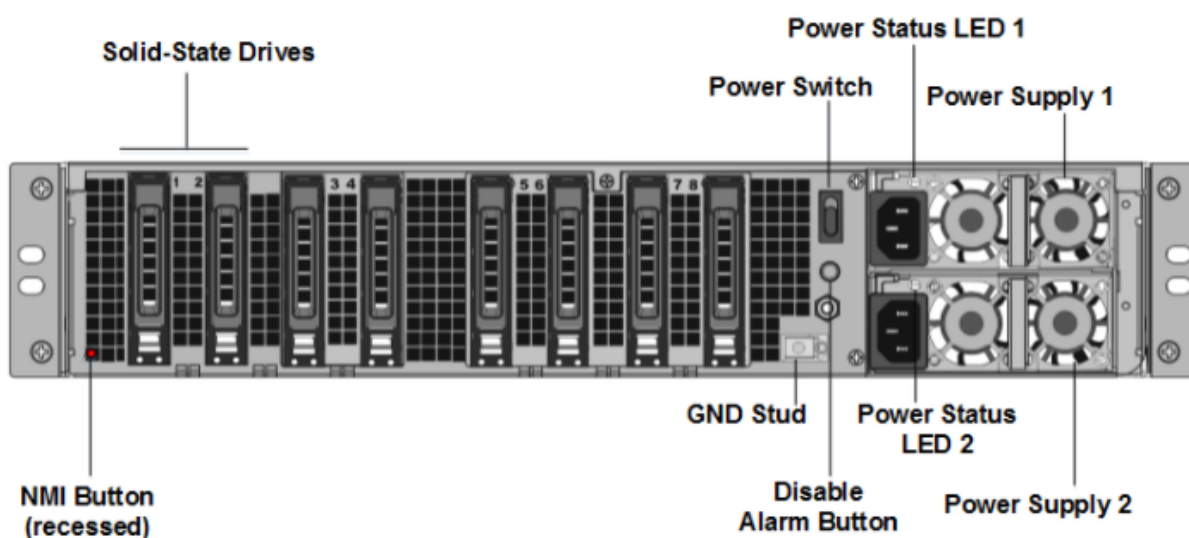

The back panel of the SDX 15000-50G appliance has the following components:

- Two 240 GB RAID-supported removable boot solid-state drives (SSDs), (slots 1 and 2) as shown in figure 2. Two 240 GB RAID-supported removable storage repositories (slots 3 and 4 paired) SSDs, and four 480 GB storage repositories (slots 5–6 paired and 7–8 paired) SSDs.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

- A power switch, which turns power to the appliance on or off. If the OS is functional, press the switch for less than two seconds to power down the system with a graceful shutdown. If the OS is not responsive, press the power switch for more than 4 seconds to force the power off.
- Two hot-swappable 100–240 VAC input power supply modules. Each power supply has an LED indicating its status, as shown in the following table.

LED Color	LED Indicates
OFF	No power to any power supply in the appliance.
Flashing RED	No power to this power supply module.
Flashing GREEN	Power supply is in standby mode.
GREEN	Power supply is functional.
RED	Power supply failure.
Flashing RED and GREEN	Warning (OVP/UVP/OCP/OTP/Fan); OVP = Over Voltage Protection; UVP = Under Voltage Protection; OTP = Over Temperature Protection.

- A **Disable alarm button**, which is functional only when the appliance has dual redundant, hot-swappable power supplies. Press this button to silence the power alarm when one of the two power supplies loses input power or when a power supply is malfunctioning.
- A Non-Maskable Interrupt (NMI) button, used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information about the lights out management port of the appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

Citrix ADC SDX 17500, SDX 19500, and SDX 21500


January 11, 2021

Note: This platform has reached its end of life.

The Citrix ADC models SDX 17500/19500/21500 are 2U appliances. Each model has two 6-core processors and 48 GB of memory.

The following figure shows the front panel of the SDX 17500/19500/21500 appliance.

Figure 1. Citrix ADC SDX 17500/19500/21500 appliance, front panel

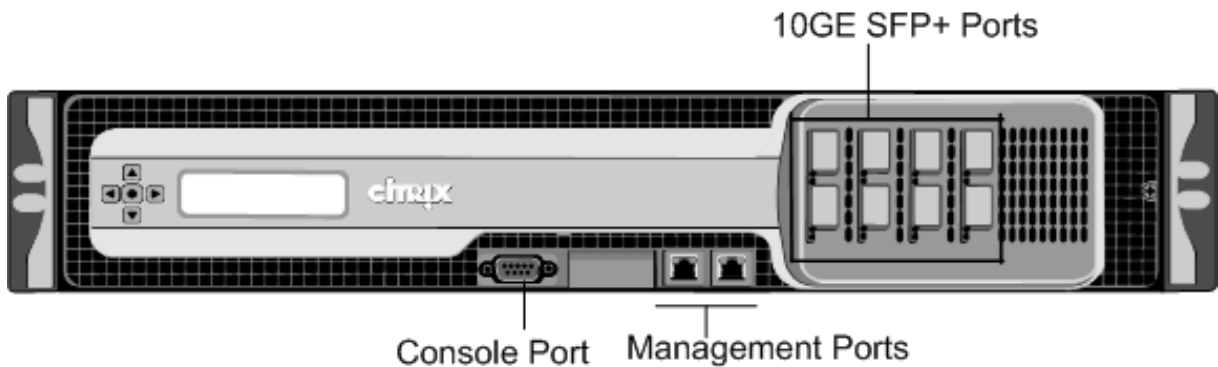


The SDX 17500/19500/21500 appliances have the following ports:

- RS232 serial console port.
- Two 10/100/1000Base-T copper Ethernet management ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Eight 10GE SFP+ ports numbered 10/1, 10/2, 10/3, and 10/4 on the top row from left to right, and 10/5, 10/6, 10/7, and 10/8 on the bottom row from left to right.

The following figure shows the back panel of the SDX 17500/19500/21500 appliance.

Figure 2. Citrix ADC SDX 17500/19500/21500 appliance, back panel

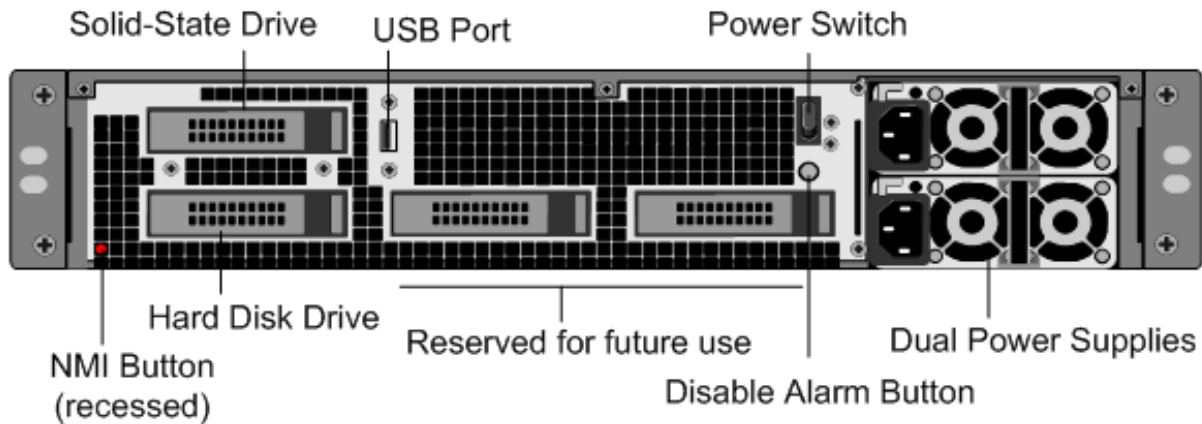

The following components are visible on the back panel of the SDX 17500/19500/21500 appliance:

- One 160 GB or larger removable solid-state drive that is used to store the Citrix ADC software.
Note: Drive densities might increase as components become EOL but its size is never smaller than the original.
- USB port (reserved for a future release).
- Power switch, which turns off power to the appliance, as if you were to unplug the power supply. Press the switch for five seconds to shut off the power.

- Non-maskable interrupt (NMI) button that is used at the request of Technical Support and produces a core dump on the Citrix ADC appliance. Use a pen, pencil, or other pointed object to press this red button, which is recessed to prevent unintentional activation.
- Removable hard-disk drive that stores user data.
- **Disable alarm button.** This button is functional only when the appliance has two power supplies.

Press this button to stop the power alarm from sounding when either of the following conditions is true:

- You have plugged the appliance into only one power outlet.
 - One power supply is malfunctioning, and you want to continue operating the appliance until it is repaired.
- Dual power supplies, each rated at 650 watts, 110–220 volts.

Citrix ADC SDX 17550, SDX 19550, SDX 20550, and SDX 21550


January 11, 2021

Note: This platform has reached its end of life.

The Citrix ADC models SDX 17550, SDX 19550, SDX 20550, and SDX 21550 are 2U appliances. Each model has two 6-core processors for a total of 12 physical cores (24 cores with hyper-threading), and 96 GB of memory.

The following figure shows the front panel of the SDX 17550/19550/20550/21550 appliance.

Figure 1. Citrix ADC SDX 17550/19550/20550/21550 appliance, front panel

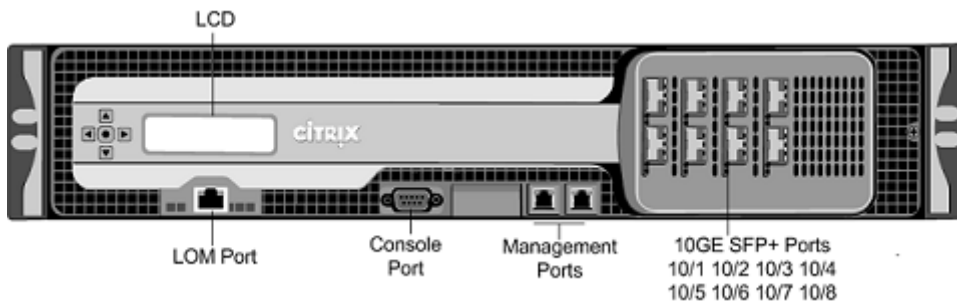

The SDX 17550/19550/20550/21550 appliance has the following ports:


- 10/100Base-T copper Ethernet Port (RJ45), also called LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.

Note: The LEDs on the LOM port are not operational by design.

- RS232 serial console port.
- Two 10/100/1000Base-T copper Ethernet management ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Eight 10GE SFP+ ports numbered 10/1, 10/2, 10/3, and 10/4 on the top row from left to right, and 10/5, 10/6, 10/7, and 10/8 on the bottom row from left to right.

The following figure shows the back panel of the SDX 17550/19550/20550/21550 appliance.

Figure 2. Citrix ADC SDX 17550/19550/20550/21550 appliance, back panel

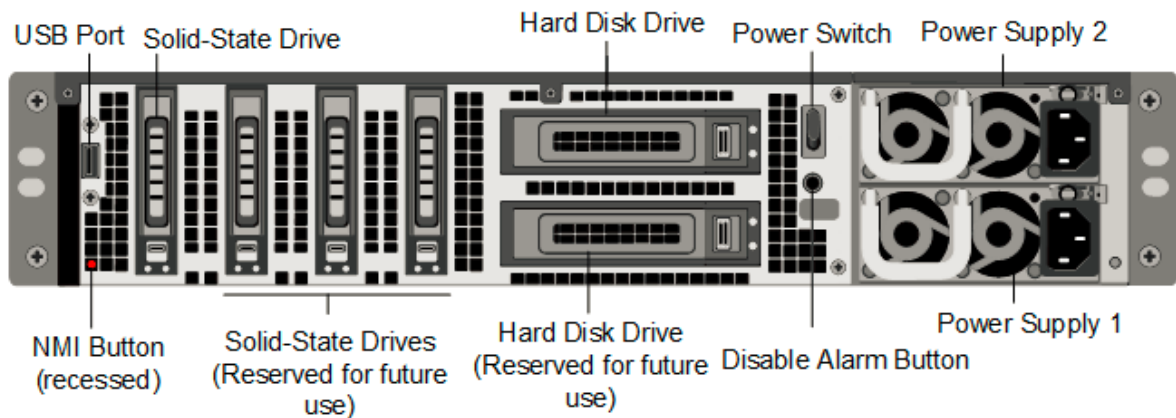

The following components are visible on the back panel of the SDX 17550/19550/20550/21550 appliance:

- One 160 GB or larger removable solid-state drive that is used to store the Citrix ADC software.
 - Note:** Drive densities might increase as components become EOL but its size is never smaller than the original.
- USB port (reserved for a future release).
- Power switch, which turns off power to the appliance, as if you were to unplug the power supply. Press the switch for five seconds to shut off the power.
- Non-maskable interrupt (NMI) button that is used at the request of Technical Support and produces a core dump on the Citrix ADC appliance. Use a pen, pencil, or other pointed object to press this red button, which is recessed to prevent unintentional activation.
- Two removable hard-disk drives that store user data.
- **Disable alarm button.** This button is functional only when the appliance has two power supplies.

Press this button to stop the power alarm from sounding when either of the following conditions is true:

- You have plugged the appliance into only one power outlet.
 - One power supply is malfunctioning, and you want to continue operating the appliance until it is repaired.
- Dual power supplies, each rated at 850 watts, 110–220 volts.

Citrix ADC SDX 22040, SDX 22060, SDX 22080, SDX 22100, and SDX 22120

August 18, 2020

The Citrix ADC


SDX 22040/22060/22080/22100/22120 are 2U appliances. Each model has two 8-core processors (32 cores with hyper-threading) and 256 GB of memory. The

SDX 22040/22060/22080/22100/22120 appliances are available in two port configurations:

- Twelve 1G SFP ports and twenty-four 10G SFP+ ports (12x1G SFP + 24x10G SFP+)
- Twenty-four 10G SFP+ ports (24x10G SFP+)


The following figure shows the front panel of the SDX 22040/22060/22080/22100/22120 (12x1G SFP + 24x10G SFP+) appliance.

Figure 1. Citrix ADC SDX 22040/22060/22080/22100/22120 (12x1G SFP + 24x10G SFP+), front panel

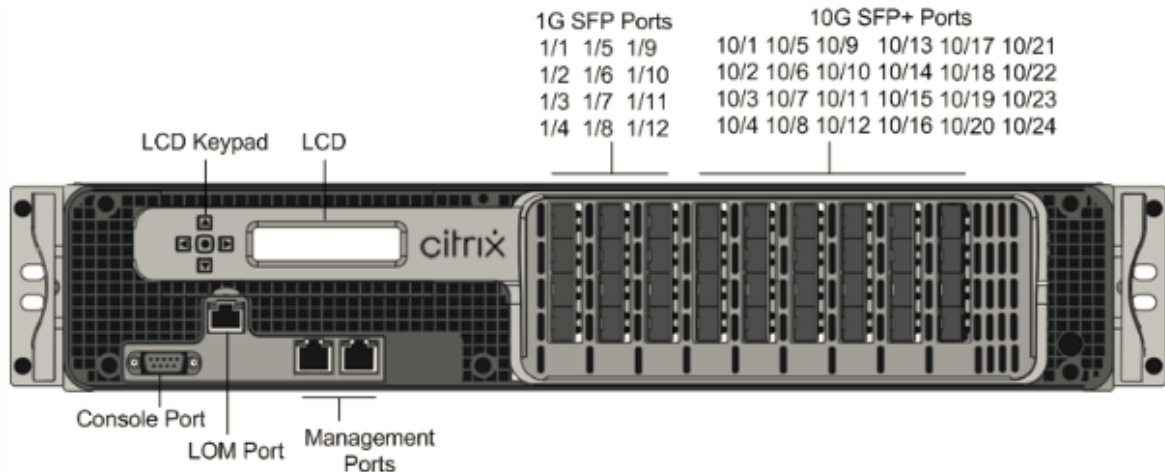

The following figure shows the front panel of the SDX 22040/22060/22080/22100/22120 (24x10G SFP+) appliance.

Figure 2. Citrix ADC SDX 22040/22060/22080/22100/22120 (24x10G SFP+), front panel

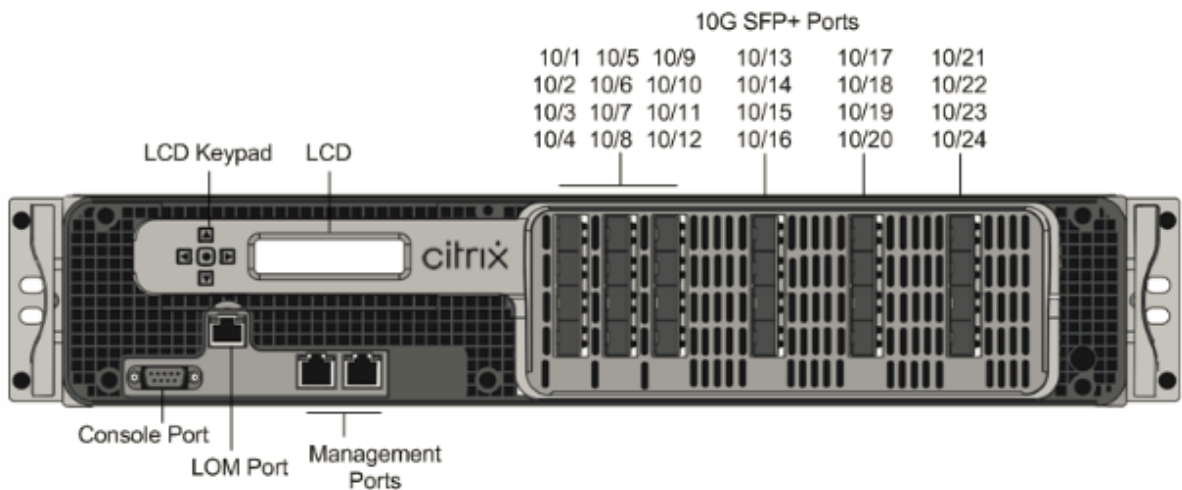


Depending on the model, the appliance has the following ports:

- RS232 serial Console Port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T copper Ethernet Management Ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Network Ports
 - SDX 22040/22060/22080/22100/22120 (12x1G SFP + 24x10G SFP+). Twelve copper or fiber 1G SFP ports and twenty-four 10G SFP+ ports.
 - SDX 22040/22060/22080/22100/22120 (24x10G SFP+). Twenty-four 10G SFP+ ports.

The following figure shows the back panel of the SDX 22040/22060/22080/22100/22120 appliances.

Figure 3. Citrix ADC SDX 22040/22060/22080/22100/22120, back panel

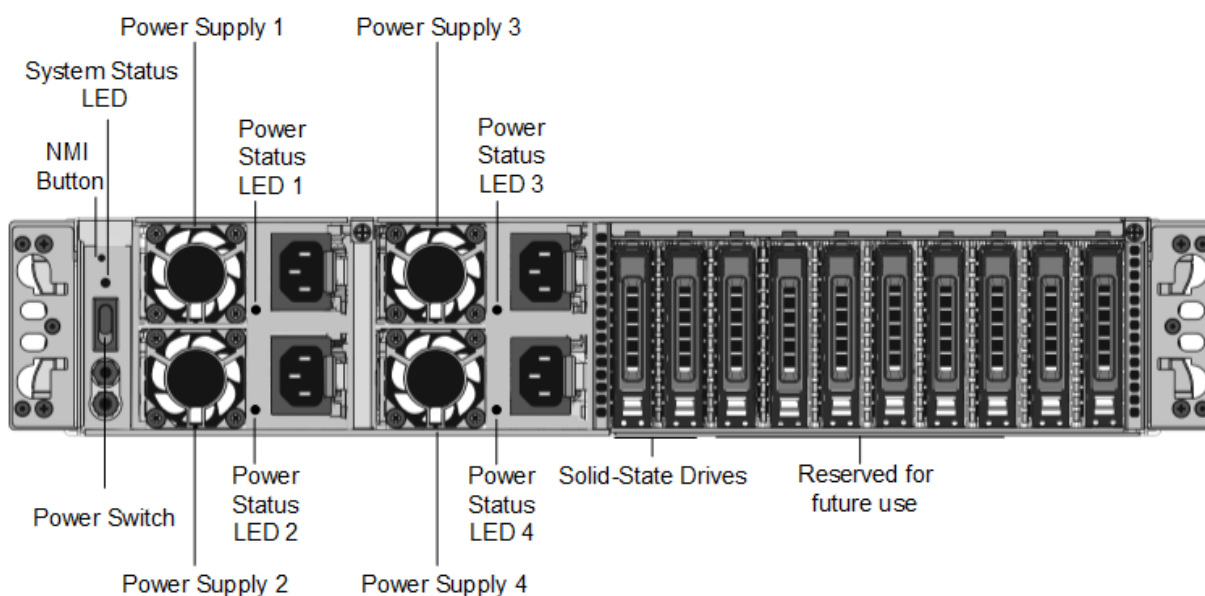

The following components are visible on the back panel of the SDX 22040/22060/22080/22100/22120 appliance:

- Non-maskable interrupt (NMI) Button, used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu.
- System status LED, which indicates the status of the appliance, as described in [LCD Display and LED Status Indicators](#).

Note: On an SDX 22040/22060/22080/22100/22120 appliance running LOM firmware version 3.22, the system status LED indicates an error (continuously glows RED) even though the appliance is functioning properly.

- Four power supplies, each rated at 750 watts, 100–240 volts. A minimum of two power supplies are required for proper operation. The extra power supplies act as backup. Each power supply has an LED that indicates the status of the power supply, as described in [LCD Display and LED Status Indicators](#).
- Power switch, which turns off power to the appliance. Press the switch for less than two seconds to shut off the power.
- One 256 GB or larger removable solid-state drive.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.


Citrix ADC SDX 24100 and SDX 24150

August 29, 2020

The Citrix ADC SDX 24100/24150 are 2U appliances. Each model has two 8-core processors (32 cores with hyper-threading) and 256 GB of memory. The SDX 24100/24150 appliances are available in the twelve 1G SFP ports and twenty-four 10G SFP+ ports (12x1G SFP + 24x10G SFP+) configuration.

The following figure shows the front panel of the SDX 24100/24150 (12x1G SFP + 24x10G SFP+) appliance.

Figure 1. Citrix ADC SDX 24100/24150 (12x1G SFP + 24x10G SFP+), front panel

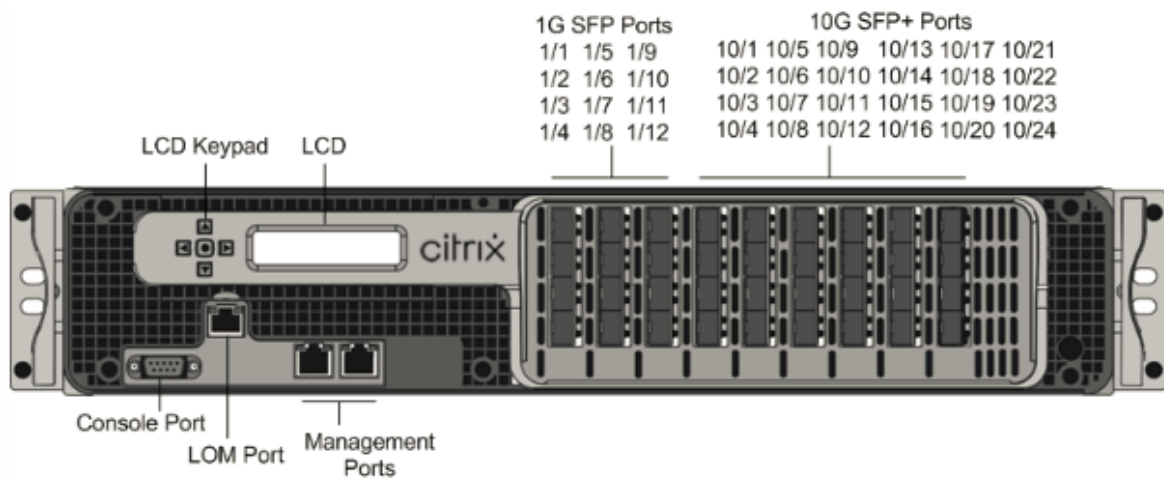


Depending on the model, the appliance has the following ports:

- RS232 serial Console Port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T copper Ethernet Management Ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Network Ports
 - SDX 24100/24150 (12x1G SFP + 24x10G SFP+). Twelve copper or fiber 1G SFP ports and twenty-four 10G SFP+ ports.

The following figure shows the back panel of the SDX 24100/24150 appliances.

Figure 2. Citrix ADC SDX 24100/24150, back panel

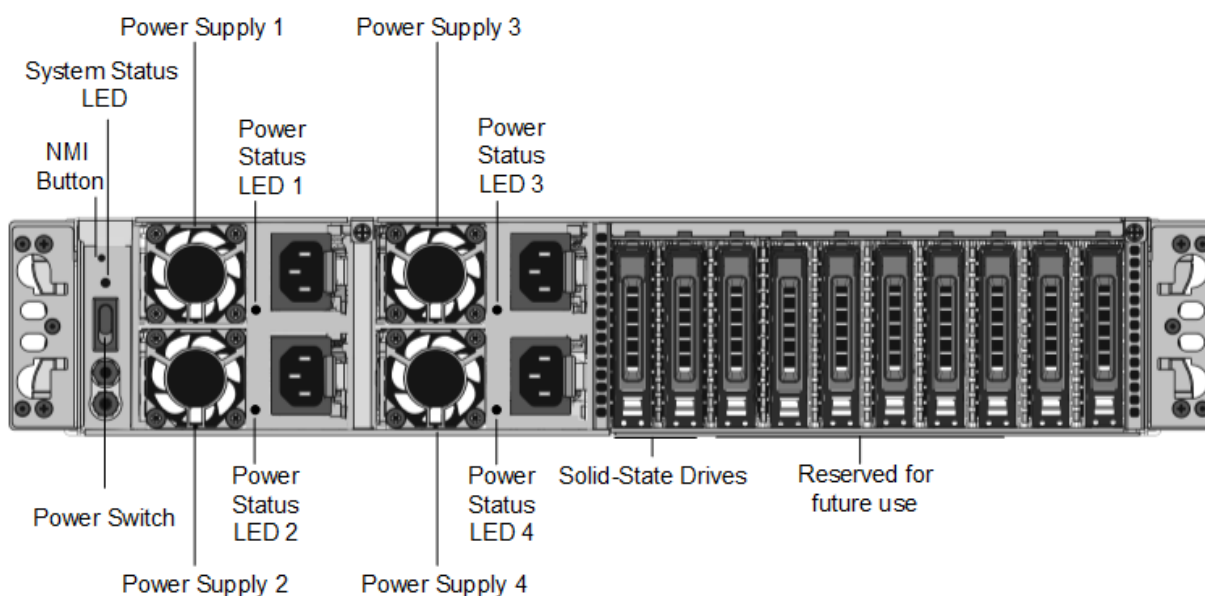

The following components are visible on the back panel of the SDX 24100/24150 appliance:

- Non-maskable interrupt (NMI) Button, used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu.
- System status LED, which indicates the status of the appliance, as described in [LCD display and LED status indicators](#).

Note: On an

SDX 24100/24150 appliance running LOM firmware version 3.22, the system status LED indicates an error (continuously glows RED) even though the appliance is functioning properly.

- Four power supplies, each rated at 750 watts, 100–240 volts. A minimum of two power supplies are required for proper operation. The extra power supplies act as backup. Each power supply has an LED that indicates the status of the power supply, as described in [LCD display and LED status indicators](#).
- Power switch, which turns off power to the appliance. Press the switch for less than two seconds to shut off the power.
- Four 600 GB removable solid-state drives. The first two leftmost solid-state drives store the Citrix ADC software. The next two solid-state drives store user data. Also, you can extend the SSD storage (optional) by another two or four 600 GB SSDs.


Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

Citrix ADC SDX 25100A, SDX 25160A

August 19, 2020

The Citrix ADC SDX 25100A and SDX 25160A are 2U appliances. Each model has two 10-core processors, 256 GB of memory, eight 40GE QSFP+ ports (8x40GE QSFP+).

Figure 1. Citrix ADC SDX 25100A and SDX 25160A front panel

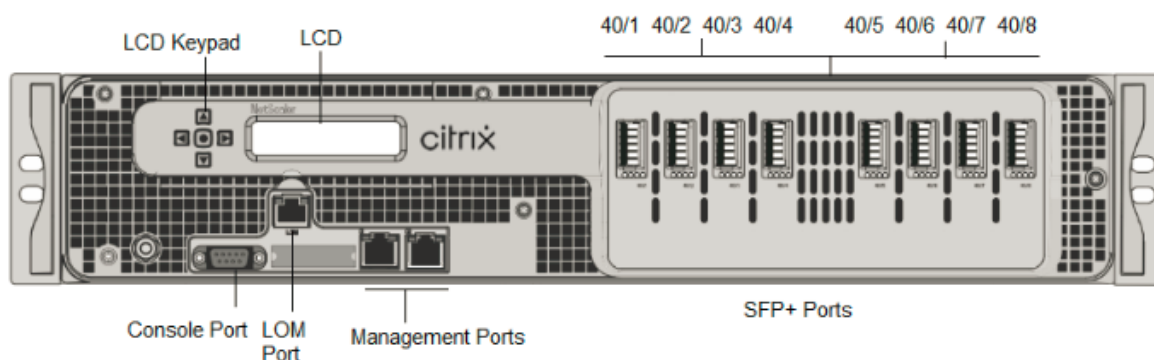


The Citrix ADC SDX 25160A and SDX 25100A appliances have the following ports:

- RS232 serial Console Port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Network ports, eight 40G QSFP+ ports.

Note

40G ports do not support 10G and 1G transceivers.

Figure 2. Citrix ADC SDX 25100A and SDX 25160A back panel

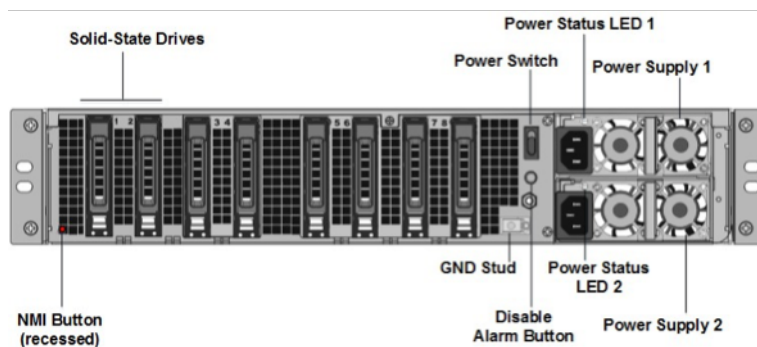

The following components are visible on the back panel of the SDX 25100A and SDX 25160A appliance:

- **Two 300 GB removable solid-state drives (SSDs).** The two leftmost solid-state drives store the Citrix ADC software. The next two solid-state drives store user data. The remaining four solid-state drives are reserved for future use. These appliances are a redundant array of independent

disks (RAID) devices.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.


- **Power switch.** Which turns power to the appliance on or off. Press the switch for less than two seconds to shut off the power.
- **Two power supplies.** each rated at 1000 watts, 100–240 volts. Each power supply has an LED that indicates the status of the power supply.
- ****Disable alarm button**.** Which is functional only when the appliance has dual redundant, hot-swappable power supplies. Press this button to silence the power alarm when one of the two power supplies loses input power or when a power supply is malfunctioning.
- **Non-maskable interrupt (NMI) button.** Used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information about the lights out management port of the appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

Citrix ADC SDX 25100-40G

August 19, 2020

The Citrix ADC SDX 25100-40G and SDX 25160-40G are 2U appliances. Each model has two 10-core processors, 256 GB of memory, four 40G QSFP+ ports, and sixteen 10G SFP+ ports (4x40G QSFP+ + 16x10G SFP+).

Figure 1. Citrix ADC SDX 25100 40G, SDX 25160 40G (4x40G QSFP+ + 16x10G SFP+) front panel

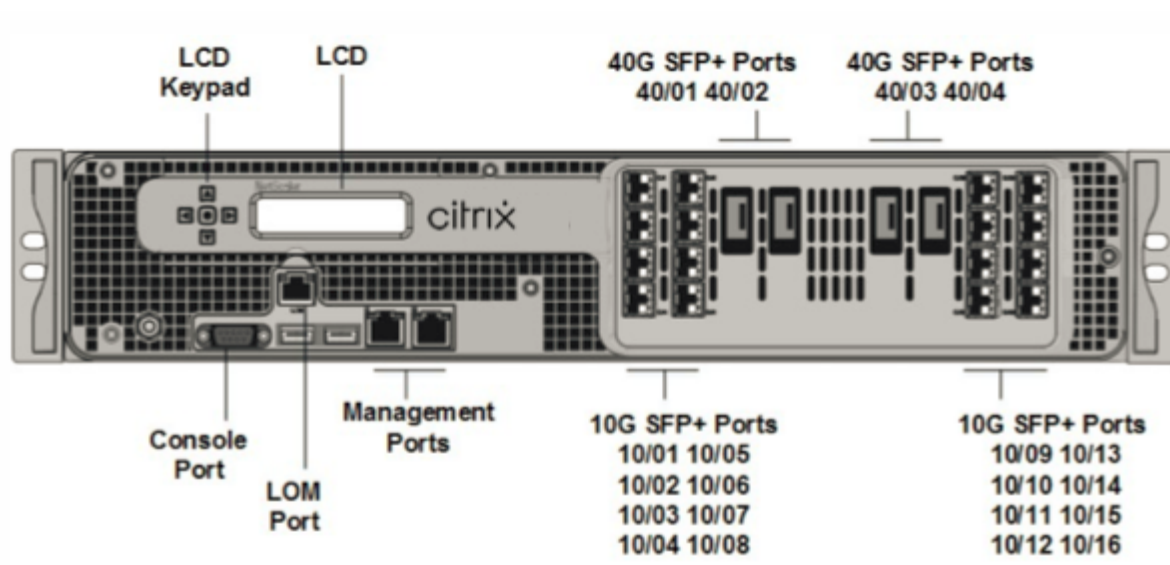


The Citrix ADC SDX 25100 40G, SDX 25160 40G appliances have the following ports:

- RS232 serial Console Port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T copper Ethernet Management Ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions.
- Network Ports: four 40G QSFP+ ports and sixteen 10G SFP+ ports (4x40G QSFP+ + 16x10G SFP+).
- USB ports (reserved for a future release).

Note:

- 10G ports do not support 1G copper or 1G fiber transceivers.
- 40G ports do not support 10G and 1G transceivers.

Figure 2. Citrix ADC SDX 25100-40G and SDX 25160-40G back panel

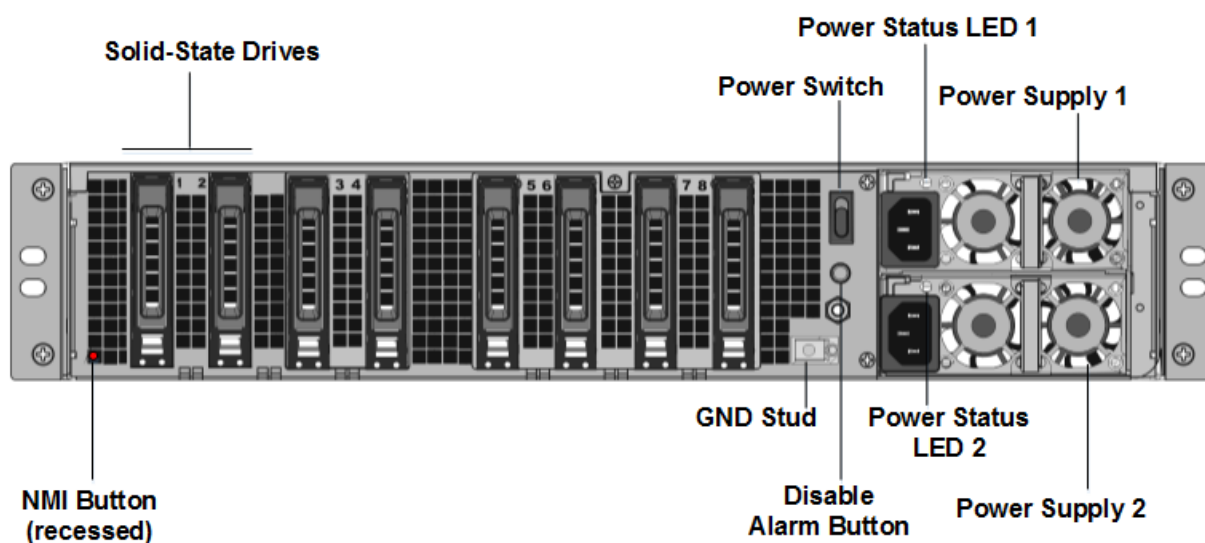

The following components are visible on the back panel of the SDX 25100-40G, SDX 25160-40G appliance:

- **Two 300 GB removable solid-state drives (SSDs).** The two leftmost solid-state drives store the Citrix ADC software. The next two solid-state drives, of 300 GB each, store user data. The remaining four solid-state drives are reserved for future use.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

- **Power switch.** Which turns power to the appliance on or off. Press the switch for less than two seconds to shut off the power.
- **Two power supplies.** Each rated at 1000 watts, 100–240 volts. Each power supply has an LED that indicates the status of the power supply, as described in [Common Hardware Components](#) [../common-hardware-components.html].
- ****Disable alarm button**.** Which is functional only when the appliance has dual redundant, hot-swappable power supplies. Press this button to silence the power alarm when one of the two power supplies loses input power or when a power supply is malfunctioning.
- **Non-maskable interrupt (NMI) button.** Used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information about the lights out management port of the appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

Citrix ADC SDX 26000


August 18, 2020

The Citrix ADC SDX 26000 appliances are 2U appliances. These appliances have two 14-core processors and 256 GB of memory. The appliance has eight 50G and sixteen 25G network ports.

For information about the software releases supported on the Citrix ADC hardware platforms, see [Citrix ADC SDX hardware-software compatibility matrix](#).

The following figure shows the front panel of the Citrix ADC SDX 26000 appliances.

Figure 1. Citrix ADC SDX 26000, front panel

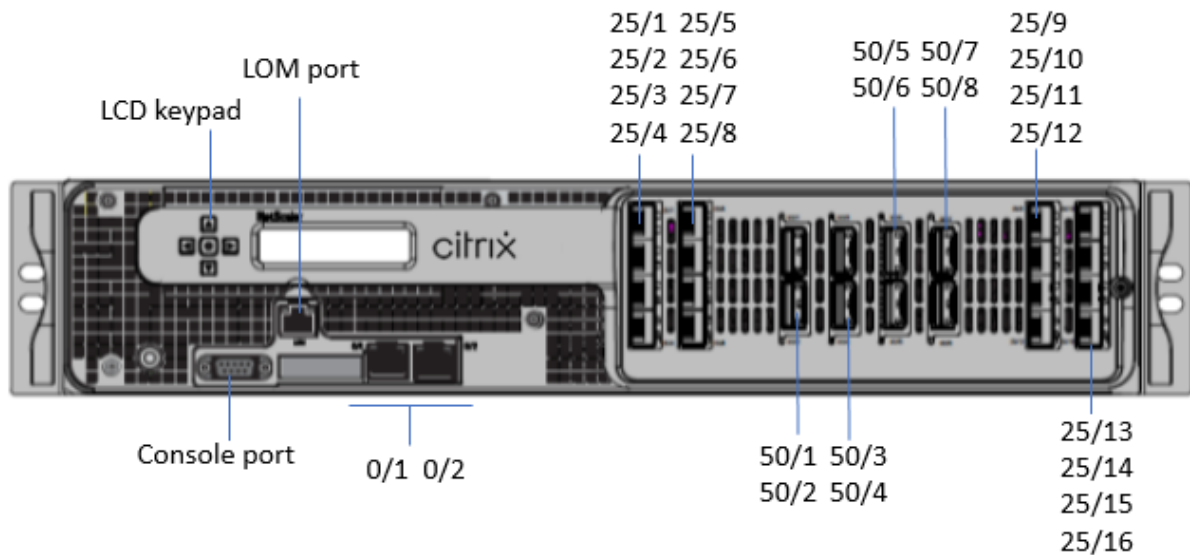


The Citrix ADC SDX 26000 appliances have the following ports:

- RS232 serial console port.
- One 10/100/1000Base-T RJ45 copper Ethernet LOM Port. Use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T RJ45 copper Ethernet Management Ports, numbered 0/1 and 0/2. These ports are used to connect directly to the appliance for Citrix ADC administration functions.
- Eight 50G ports, numbered 50/1 to 50/8.
- Sixteen 25G ports, numbered 25/1 through 25/16.

The following figure shows the back panel of the SDX 26000 appliances.

Figure 2. Citrix ADC SDX 26000, back panel

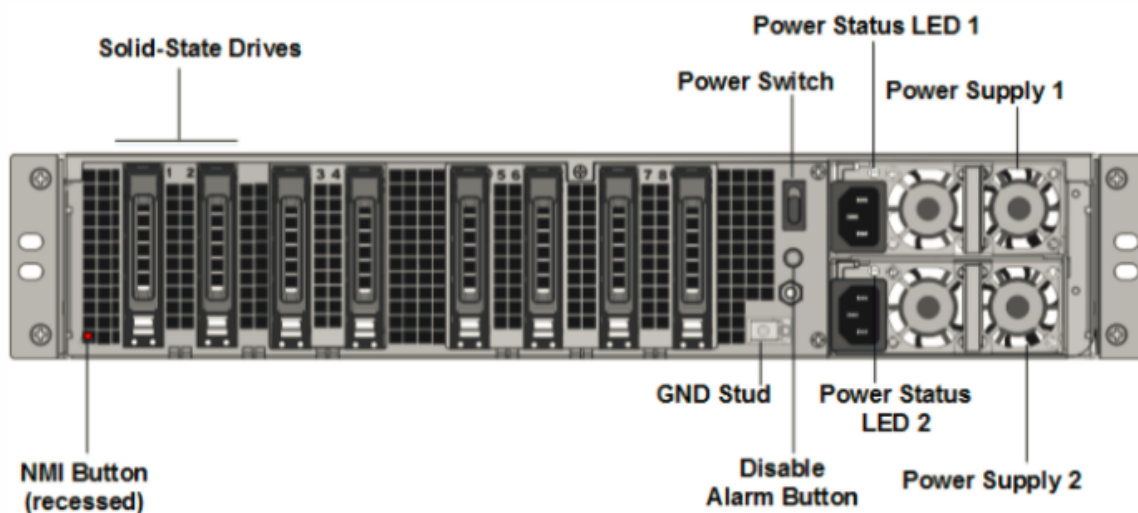

The following components are visible on the back panel of the Citrix ADC SDX 26000 appliances:

- Two 240 GB and six 960 GB removable solid-state drive (SSD).
 - Note:** Drive densities might increase as components become EOL but its size is never smaller than the original.
- Power switch, which turns power to the appliance on or off.
 - If the OS is functional, press the switch for less than two seconds to power down the system with a graceful shutdown.
 - If the OS is not responsive, press the power switch for more than 4 seconds to force the power off.
- Two hot-swappable 100–240 VAC, 1000 W power supply modules. Max power consumption is 672 W. Typical power consumption is 540 W. Each power supply has an LED indicating its status as follows:

LED Color	LED Indicates
OFF	No power to any power supply on the appliance.
Flashing RED	No power to this power supply.
Flashing GREEN	Power supply is in standby mode.
GREEN	Power supply is functional.
RED	Power supply failure.

LED Color	LED Indicates
Flashing RED and GREEN	Warning (OVP/UVP/OCP/OTP/Fan); OVP = Over Voltage Protection; UVP = Under Voltage Protection; OCP = Over Current Protection; OTP = Over Temperature Protection

- **Disable alarm button.** Press this button to silence the power alarm when one of two power supplies loses input power or when a power supply is malfunctioning.
- **Non-Maskable Interrupt (NMI) Button,** used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information, see [Lights out management port of the Citrix ADC SDX appliance.](#)

Citrix ADC SDX 26000-50S


August 18, 2020

The Citrix ADC SDX 26xxx-50S appliances are 2U appliances. These appliances have two 14-core processors and 256 GB of memory. The appliances have four 50G and sixteen 25G network ports.

For information about software releases supported on the Citrix ADC hardware platforms, see [Citrix ADC SDX hardware-software compatibility matrix.](#)

The following figure shows the front panel of the Citrix ADC SDX 26xxx-50S appliances.

Figure 1. Citrix ADC SDX 26xxx-50S, front panel

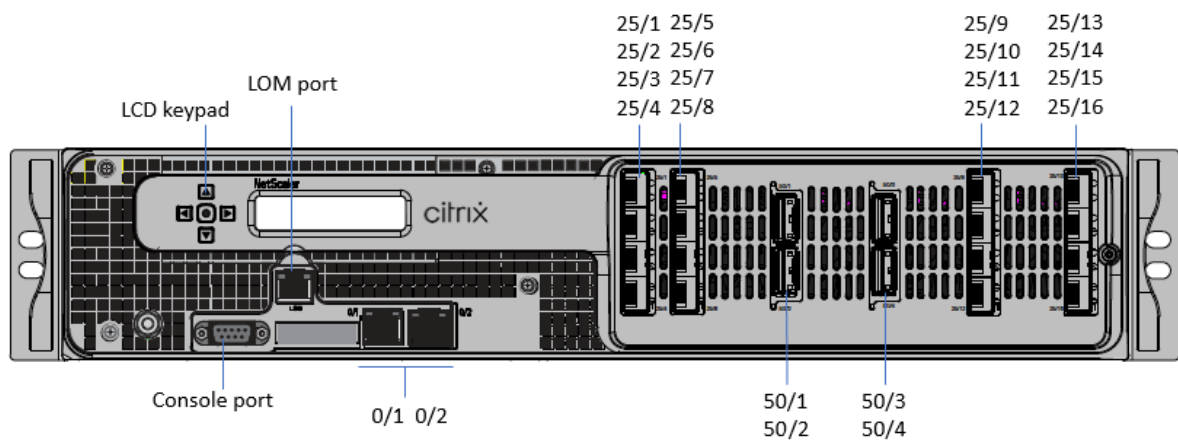


The Citrix ADC SDX 26xxx-50S appliances have the following ports:

- RS232 serial console port.
- One 10/100/1000Base-T RJ45 copper Ethernet LOM Port. Use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T RJ45 copper Ethernet Management Ports, numbered 0/1 and 0/2. These ports are used to connect directly to the appliance for Citrix ADC administration functions.
- Four 50G ports, numbered 50/1 to 50/4.
- Sixteen 25G ports, numbered 25/1 through 25/16.

The following figure shows the back panel of the SDX 26xxx-50S appliances.

Figure 2. Citrix ADC SDX 26xxx-50S, back panel

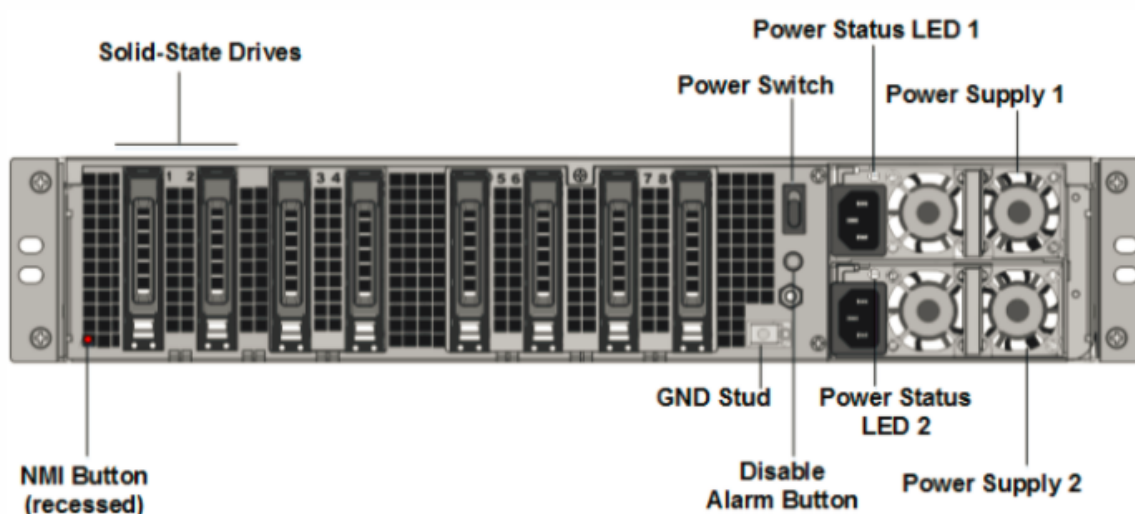

The following components are visible on the back panel of the Citrix ADC SDX 26xxx-50S appliances:

- Two 240GB and six 960GB removable solid-state drive (SSD).
 - Note:** Drive densities might increase as components become EOL but its size is never smaller than the original.
- Power switch, which turns power to the appliance on or off.
 - If the OS is functional, press the switch for less than two seconds to shut down gracefully.
 - If the OS is not responsive, press the power switch for more than 4 seconds, for a hard shutdown.
- Two hot-swappable 100–240 VAC, 1200 W power supply modules. Max power consumption is 764 W. Typical power consumption is 628 W. Each power supply has an LED indicating its status:

LED Color	LED Indicates
OFF	No power to any power supply on the appliance.
Flashing RED	No power to this power supply.
Flashing GREEN	Power supply is in standby mode.
GREEN	Power supply is functional.
RED	Power supply failure.
Flashing RED and GREEN	Warning;(OVP/UVP/OCP/OTP/Fan); OVP = Over Voltage Protection; UVP = Under Voltage Protection; OCP = Over Current Protection; OTP = Over Temperature Protection

- **Disable alarm button.** Press this button to silence the power alarm when power supply loses input power or when a power supply is malfunctioning.
- **Non-Maskable Interrupt (NMI) button:** is recessed to prevent unintentional activation and used at the request of Technical Support to start a core dump. To press this red button, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information, see [Lights out management port of the Citrix ADC SDX appliance](#).

Citrix ADC SDX 26000-100G


August 29, 2020

The Citrix ADC SDX 26000-100G appliance is a 2U appliance. This platform has two 14-core processors and 256 GB memory. The appliance provides a total of 8 network ports.

For information about the software releases supported on the Citrix ADC hardware platforms, see [Citrix ADC SDX Hardware-Software Compatibility Matrix\]\(../supported-versions.html\)](#).

The illustrations in this guide are only indicative and might not represent the actual Citrix ADC appliance.


Figure 1. Citrix ADC SDX 26000-100G front panel

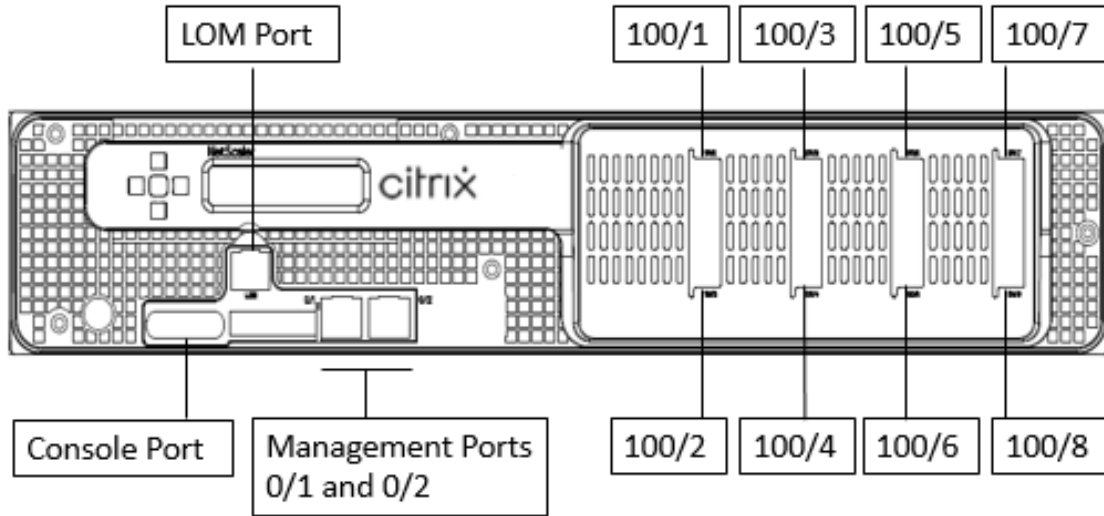

The Citrix ADC SDX 26000-100G appliances have the following ports:

- RS232 serial Console Port.
- One 10/100/1000Base-T RJ45 copper Ethernet LOM Port. Use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.
- Two 10/100/1000Base-T RJ45 copper Ethernet Management Ports, numbered 0/1 and 0/2. These ports are used to connect directly to the appliance for Citrix ADC administration functions.
- Eight 100G Ethernet Ports, numbered 100/1 to 100/8 from left to right. Contact Citrix support for a list of all supported 100G transceivers.

Figure 2. Citrix ADC SDX 26000-100G back panel

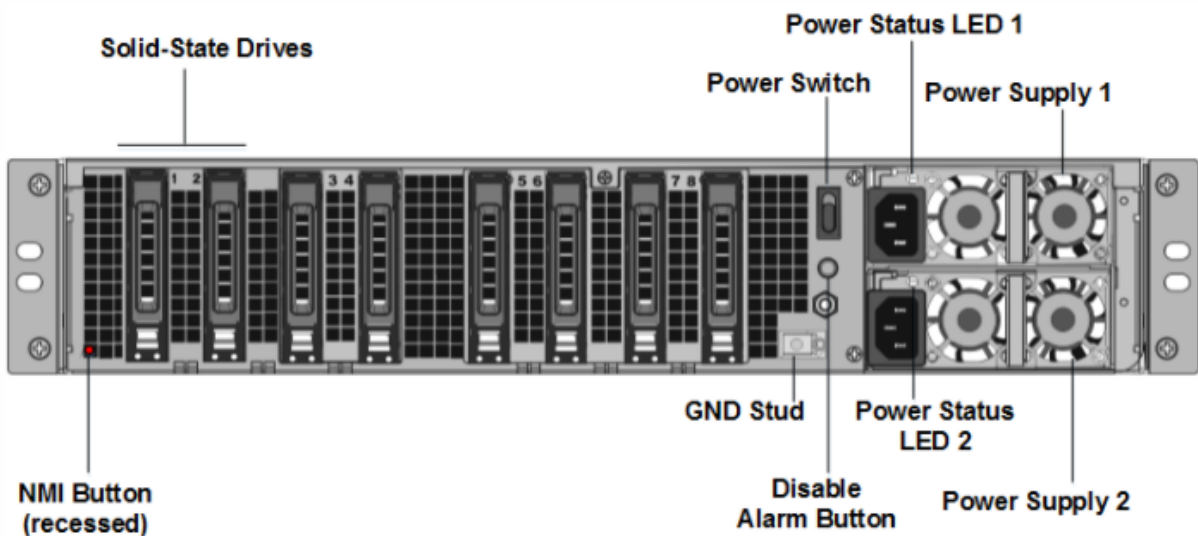

The following components are visible on the back panel of the SDX 26000-100G appliances:

- Two 240 GB removable boot solid-state drives (SSDs).
- Six 960 GB removable SSDs.

Note: Drive densities might increase as components become EOL but its size is never smaller than the original.

- Power switch, which turns power to the appliance on or off.
 - If the OS is functional, press the switch for less than two seconds to power down the system with a graceful shutdown.
 - If the OS is not responsive, press the power switch for more than 4 seconds to force the power off.
- Two power supplies, 100–240 VAC. Each power supply has an LED indicating its status, as described in the following table:

LED Color	LED Indicates
OFF	No power to any power supply on the appliance.
Flashing RED	No power to this power supply.
Flashing GREEN	Power supply is in standby mode.
GREEN	Power supply is functional.
RED	Power supply failure.
Flashing RED and GREEN	Warning (OVP/UVP/OCP/OTP/Fan); OVP = Over Voltage Protectio; UVP = Under Voltage Protection; OCP = Over Current Protection; OTP = Over Temperature Protection.

- **Disable alarm button**, which is functional only when the appliance has dual redundant, hot-swappable power supplies. Press this button to silence the power alarm when one of the two power supplies loses input power or when a power supply is malfunctioning.
- Non-Maskable Interrupt (NMI) Button, used at the request of Technical Support to initiate a core dump. To press this red button, which is recessed to prevent unintentional activation, use a pen, pencil, or other pointed object. The NMI Button is also available remotely over the network in the LOM GUI, in the Remote Control menu. For more information about the lights out management port of the appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

Common hardware components

May 4, 2021

Each platform has front panel and back panel hardware components. The front panel has an LCD display and an RS232 serial console port. The number, type, and location of ports—copper Ethernet, copper and fiber 1G SFP, 10GSFP+, and 40G QSFP+. The back panel provides access to the fan and the field replaceable units (power supplies, CompactFlash card, and solid-state and hard-disk drives).

LCD display and LED status indicators

On some Citrix ADC SDX appliances, the LCD on the front panel displays the appliance's model number, but the number shown might not be the licensed model number. To view the licensed model number of any SDX appliance, log on to the Management Service and check the licensed model number in the top left corner of the screen. For example, if you have purchased an SDX 11515 license, the LCD screen displays CITRIX NSSDX-11500, and the Management Service screen displays Citrix ADC SDX (11515).

The LCD backlight on the Citrix ADC appliance is always on.

On the appliance's back panel, system status LEDs indicate the overall status of the appliance. The following table describes the indicators of the system status LED.

On the appliance's back panel, power status LEDs indicate the status of each power supply.

Note

System status LEDs are available on only some Citrix ADC SDX appliances.

LED Color	LED Indicates
OFF	No power
Green	Appliance is receiving power
Red	Appliance has detected an error

The port LEDs show whether a link is established and traffic is flowing through the port. The following table describes the LED indicators for each port. There are two LED indicators for each port type.

Note

This section applies to all the appliances.

LED port-status indicators

Port type	LED color	LED indicates
50 Gbps	Off	A link has not been established
	Blinking amber	Indicates a problem with the link
	Solid green	Indicates a valid link with no active traffic
	Blinking green	Indicates a valid link with active traffic

Port type	LED	LED	LED color	LED indicates
10 Gbps	Top	Speed	Off	No connection.
			Solid blue	Traffic rate of 10 gigabits per second
			Off	No link
	Bottom	Link/Activity	Solid green	Link is established but no traffic is passing through the port
			Blinking green	Traffic is passing through the port
			Off	No link
1G SFP (1 Gbps)	Left	Link/Activity	Solid green	Link is established but no traffic is passing through the port
			Blinking green	Traffic is passing through the port
			Off	No link
	Right	Speed	Off	No connection

Port type	LED	LED	LED color	LED indicates
			Yellow	Traffic rate of 1 gigabit per second
Management (RJ45)	Left	Speed	Off	No connection, or a traffic rate of 10 megabits per second (Mbps)
			Green	Traffic rate of 100 Mbps
			Amber	Traffic rate of 1 gigabit per second
	Right	Link/Activity	Off	No link
			Solid yellow	Link is established but no traffic is passing through the port

On each power supply, a bicolor LED indicator shows the condition of the power supply.

LED power supply indicators

Power supply type	LED color	LED indicates
AC	OFF	No power to any power supply
	Flashing RED	No power to this power supply
	Flashing GREEN	Power supply is in standby mode
	GREEN	Power supply is functional
	RED	Power supply failure

Ports

Ports are used to connect the appliance to external devices.

Citrix ADC appliances support RS232 serial ports, 10/100/1000Base-T copper Ethernet ports, 1-gigabit copper and fiber 1G SFP ports, 10-gigabit fiber SFP+, 25 GB, 40 GB QSFP+, 50 GB, and 100 GB ports. All Citrix ADC appliances have a combination of some or all of these ports. For details on the type and number of ports available on your appliance, see the section describing that platform.

Note

Citrix ADC appliances leverage the Receive Side Scaling (RSS) feature to optimally distribute and process traffic. The RSS implementation is based on Toeplitz hashing which distributes the packet among its queues based on the 5-tuple: TCP/IP protocol, source IP address, destination IP address, source port, and destination port.

RS232 serial port

The RS232 serial console port provides a connection between the appliance and a computer, allowing direct access to the appliance for initial configuration or troubleshooting.

All hardware platforms ship with an appropriate serial cable used to connect your computer to the appliance. For instructions on connecting your computer to the appliance, see [Installing the Hardware](#).

Copper Ethernet ports

The copper Ethernet ports installed on many models of the appliance are standard RJ45 ports.

There are two types of copper Ethernet ports that are installed on your appliance:

- 10/100BASE-T port

The 10/100BASE-T port has a maximum transmission speed of 100 megabits per second (Mbps). Most platforms have at least one 10/100BASE-T port.

- 10/100/1000BASE-T port

The 10/100/1000BASE-T port has a maximum transmission speed of 1 gigabit per second, 10 times faster than the other type of copper Ethernet port.

Most platforms have at least one 10/100/1000Base-T port.

To connect any of these ports to your network, you plug one end of a standard Ethernet cable into the port and plug the other end into the appropriate network connector.

Management ports

Management ports are standard copper Ethernet ports (RJ45), which are used for direct access to the appliance for system administration functions.

1G SFP, 10G SFP+, and 40G QSFP+ ports

A 1G SFP port can operate at a speed of 1 Gbps. It accepts either a copper 1G SFP transceiver for operation as a copper Ethernet port, or a fiber 1G SFP transceiver for operation as a fiber optic port.

The 10G SFP+ and Base-T 10G, 40G QSFP+ are high-speed ports that can operate at speeds of up to 40 Gbps. You need a fiber optic cable to connect to a port. If the other end of the fiber optic cable is attached to a 1G SFP port, the 10G SFP+ port negotiates to match the speed of the 1G SFP port.

Ports compatibility

On some appliances, the 10G slot supports **copper** 1G transceivers, which can operate at up to 1 Gbps in a 10 Gbps slot.

Note

- Certain platforms have 10G slots that do not support copper transceivers. Check with your account representative for support details.
- You cannot insert a fiber 1G transceiver into a 10G slot.
- You cannot insert a 10G transceiver into a 1G slot.


The 10G SFP+, modules are dual-speed capable and support both 1 Gbps and 10 Gbps, depending on the peer switch that the model connects to.

25G, 40G, 50G, and 100G ports

A 100G port can support five speeds: 10G, 25G, 40G, 50G, and 100G. 1G speed is not supported on the 100G port. 50G and 100G ports use the same transceiver. 40G QSFP+ are high-speed ports that can operate at speeds of up to 40 Gbps. The appliance determines the speed, and not the port.


Only 50G/100G (QSFP28) and 40G (QSFP+) transceivers can be directly used on a QSFP28 interface. Use a QSA28 adapter on a QSFP28 interface to use 10G (SFP+) and 25G (SFP28) transceivers.

The following diagram shows the transceiver compatibility.

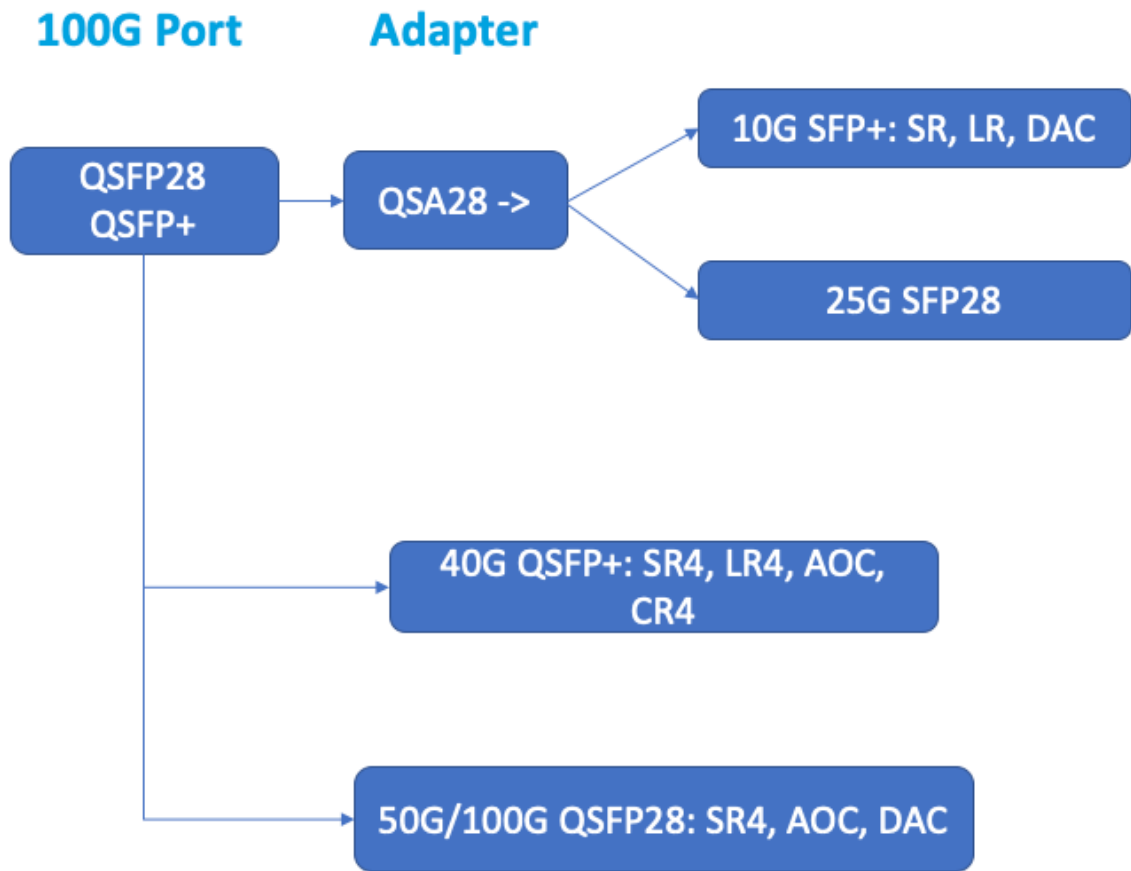


50G Port

Adapter

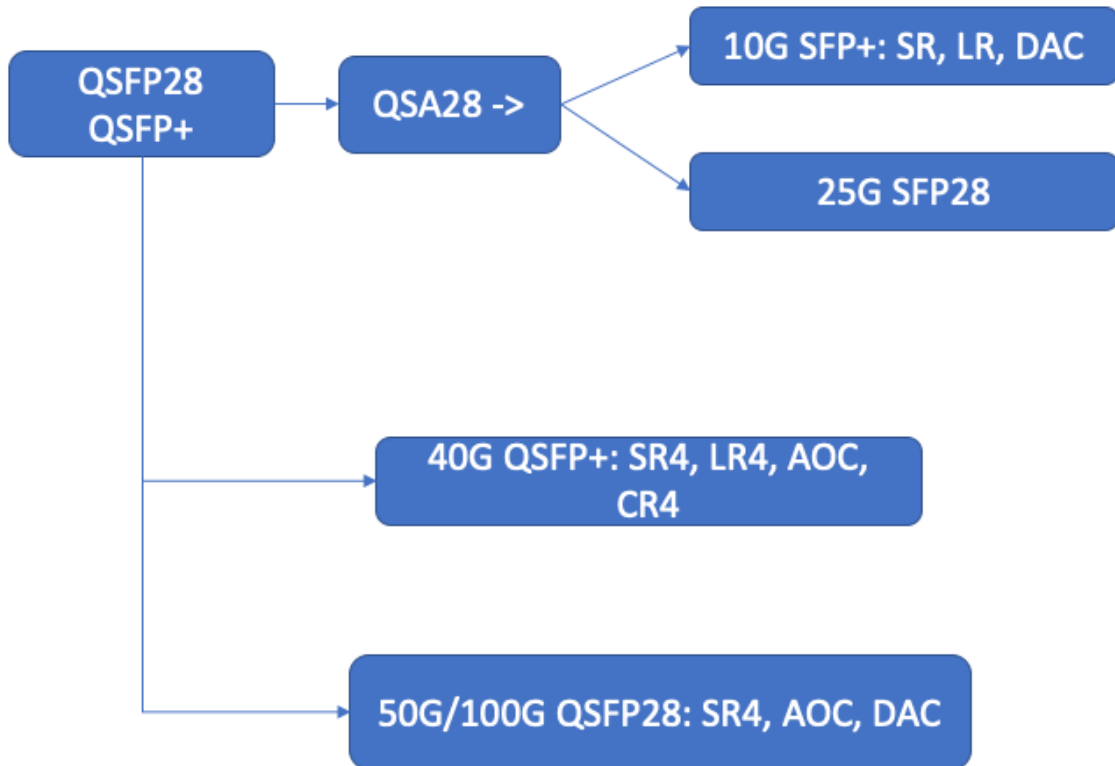

40G Port



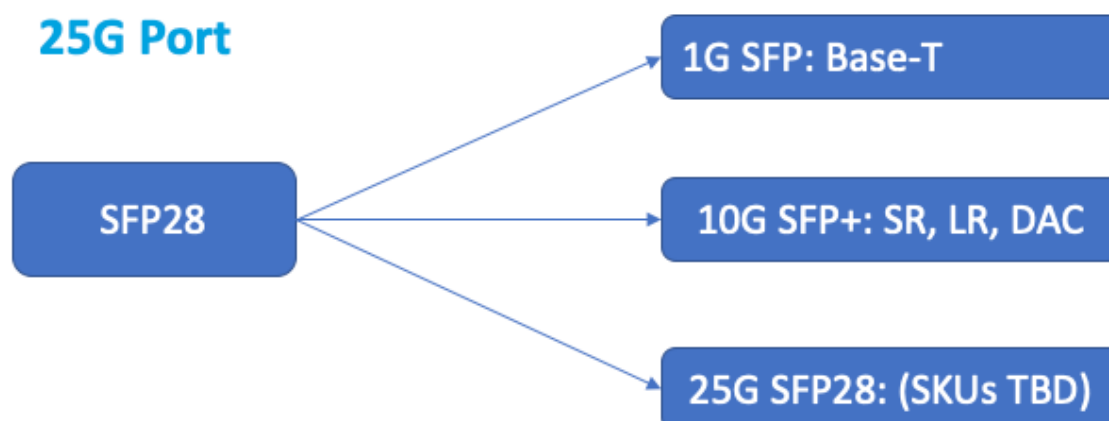

Most tables have the following columns:

- Description: The price list description of the part.
- Transmit Wavelength: The nominal transmit wavelength.
- Cable/Fiber Type: Fiber characteristics affect the maximum transmit distance achievable, especially with 10G on multi-mode fiber (MMF), where various dispersion components become dominant. For more information, see <http://www.thefoa.org/tech/ref/basic/fiber.html>.
- Typical Reach: Maximum transmit distance.
- Products: Some chassis are available with different media options. Use the appropriate data sheet to confirm that your particular chassis type supports the media.

1G pluggable media

The following table lists the maximum distance specifications for 1G transceivers.

Copper 1G SFP distance specifications

Description: Citrix ADC 1G SFP Ethernet copper (100 m) - 4 pack

Transmitter wavelength (nm): Not applicable

Cable type: Category 5 (Cat-5) copper cable

Typical reach (m): 100 m

Applicable platforms:

SDX 8015/8400/8600

SDX 14000

SDX 22040/22060/22080/22100/22120

SDX 24100/24150

Short reach fiber 1G SFP distance specifications

Description: Citrix ADC 1G SFP Ethernet SX (300 m) - 4 pack

Transmitter wavelength (nm): 850 nm (nominal)

Fiber type: 50/125um MMF, 2000MHz-km (OM3) Typical Reach (m): 550 m

Fiber type: 50/125um MMF, 500MHz-km (OM2) Typical Reach (m): 550 m

Fiber type: 50/125um MMF, 400MHz-km Typical Reach (m): 550 m

Fiber type: 62.5/125um MMF, 200MHz-km (OM1) Typical Reach (m): 300 m

Fiber type: 62.5/125um MMF, 160MHz-km Typical Reach (m): 300 m

Applicable platforms:

SDX 8015/8400/8600

SDX 22040/22060/22080/22100/22120

SDX 24100/24150

Short reach fiber 1G SFP distance specifications

Description: Citrix ADC 1G SFP Ethernet short range (300 m) - Single

Transmitter wavelength (nm): 850 nm (nominal)

Fiber type: 50/125um MMF, 2000MHz-km (OM3) Typical Reach (m): 550 m

Fiber type: 50/125um MMF, 500MHz-km (OM2) Typical Reach (m): 550 m

Fiber type: 50/125um MMF, 400MHz-km Typical Reach (m): 550 m

Fiber type: 62.5/125um MMF, 200MHz-km (OM1) Typical Reach (m): 275 m

Fiber type: 62.5/125um MMF, 160MHz-km Typical Reach (m): 220 m

Applicable platforms:

SDX 8015/8400/8600

SDX 11500/13500/14500/16500/18500/20500

SDX 11515/11520/11530/11540/11542

SDX 17500/19500/21500

SDX 22040/22060/22080/22100/22120

SDX 24100/24150

Long reach fiber 1G SFP distance specifications

Description: Citrix ADC 1G SFP Ethernet LX - Single

Transmitter wavelength (nm): 1310 nm (nominal)

Fiber type: 9/125um SMF

Typical reach (m): 10 km

Applicable platforms:

SDX 8015/8400/8600

SDX 22040/22060/22080/22100/22120

SDX 24100/24150

Long reach fiber 1G SFP distance specifications

Description: Citrix ADC 1G SFP Ethernet long range (10 km) - Single

Transmitter wavelength (nm): 1310 nm (nominal)

Fiber type: 9/125um SMF

Typical reach (m): 10 km

Applicable platforms:

SDX 8015/8400/8600

SDX 11500/13500/14500/16500/18500/20500

SDX 11515/11520/11530/11540/11542

SDX 17500/19500/21500

SDX 22040/22060/22080/22100/22120

SDX 24100/24150

10 GE pluggable media

The following table lists the maximum distance specifications for 10G transceivers.

Short reach fiber 10G SFP+ distance specifications

Description: Citrix ADC 10G SFP+, Ethernet Short Range (300 m) - Single

Transmitter wavelength (nm): 850 nm (nominal)

Fiber types

50/125um MMF, 2000MHz-km (OM3), typical reach (m): 300 m

50/125um MMF, 500MHz-km (OM2), typical reach (m): 82 m

50/125um MMF, 400MHz-km, typical reach 66 m

62.5/125um MMF, 200MHz-km (OM1), typical reach: 33 m

62.5/125um MMF, 160MHz-km, typical reach: 26 m

Applicable platforms:

- SDX 8015/8400/8600

- SDX 11500/13500/14500/16500/18500/20500
- SDX 11515/11520/11530/11540/11542
- SDX 17500/19500/21500
- SDX 22040/22060/22080/22100/22120
- SDX 24100/24150
- SDX 25000-40G
- SDX 14000
- SDX 14000-40G
- SDX 14000-40S
- SDX 14000 FIPS
- SDX 15000
- SDX 15000-50G (adapter required to connect 50G ports to 10G transceiver)
- SDX 26000 (adapter required to connect 50G ports to 10G transceiver)
- SDX 26000-50S (adapter required to connect 50G ports to 10G transceiver)
- SDX 26000-100G (adapter required to connect 100G ports to 10G transceiver)

Long reach fiber 10G SFP+ distance specifications

Description: Citrix ADC 10G SFP+ Ethernet long range (10 km) - Single

Transmitter wavelength (nm): 1310 nm (nominal)

Fiber type: 9/125um SMF

Typical reach (m): 10 km

Applicable platforms:

- SDX 8015/8400/8600
- SDX 11500/13500/14500/16500/18500/20500
- SDX 11515/11520/11530/11540/11542
- SDX 17500/19500/21500
- SDX 22040/22060/22080/22100/22120
- SDX 24100/24150
- SDX 25000-40G
- SDX 14000
- SDX 14000-40G
- SDX 14000-40S
- SDX 14000 FIPS
- SDX 15000
- SDX 15000-50G (adapter required to connect 50G ports to 10G transceiver)
- SDX 26000 (adapter required to connect 50G ports to 10G transceiver)
- SDX 26000-50S (adapter required to connect 50G ports to 10G transceiver)

- SDX 26000-100G (adapter required to connect 100G ports to 10G transceiver)

Field replaceable units

August 29, 2020

Citrix ADC field replaceable units (FRUs) are components that can be removed from the appliance and replaced by the user or a technician at the user's site. The FRUs in a Citrix ADC SDX appliance can include DC or AC power supplies, solid-state drives (SSDs), and a direct-attach cable (DAC).

Note

The figures in this section are illustrative. The actual product might vary depending on the model number.

This topic includes the following sections:

- Power Supply
- Solid-State Drive
- Direct Attach Cable

Power supply

For appliances containing two power supplies, the second power supply acts as a backup. Some appliances can accommodate four power supplies, and require two power supplies for proper operation. The third and fourth power supplies act as backup. All power supplies must be of the same type (AC or DC).

The SDX appliance ships with a country-specific power cord and a plug.

For power-supply specifications, see the [SDX hardware platforms](#) topic, which describes the various platforms.

Note

If you suspect that a power-supply fan is not working, check the system health through the SDX GUI or lights out management. For more information, see [System Health Monitoring](#) and [Lights out management port of the Citrix ADC SDX appliance](#).

On each power supply, a bicolor LED indicator shows the condition of the power supply. Green means that the appliance receives power. Red means that the power supply has detected an error. For more information about the LED power supply indicator, see "LCD Display and LED Status Indicators" in [Common hardware components](#).

Electrical Safety Precautions for Power Supply Replacement

- Ensure that the appliance has a direct physical connection to earth ground during normal use. When installing or repairing an appliance, always connect the ground circuit first and disconnect it last.
- Citrix ADC SDX appliances do not contain user serviceable components, except as noted in the (FRU) section. Do not attempt to open the chassis.
- Always unplug the power cord from the power source before removing the power supply.
- Never touch a power supply when the power cord is plugged in. As long as the power cord is plugged in, line voltages are present in the power supply even if the power switch is turned off.

For the complete list of safety precautions, see [Safety, cautions, warnings, and other information](#).

Replace an AC or a DC power supply

If the appliance has only one power supply, you have to shut down the appliance before replacing the power supply. If the appliance has two power supplies, you can replace one power supply without shutting down the appliance, provided the other power supply is working.

To install or replace an AC or a DC power supply on a Citrix ADC SDX appliance

1. Align the semicircular handle perpendicular to the power supply. Loosen the thumbscrew and press the lever toward the handle and pull out the existing power supply, as shown in the following figure.

Figure 1. Remove an Existing AC Power Supply



Figure 2. Remove an Existing DC Power Supply



2. Carefully remove the new power supply from its box.
3. On the back of the appliance, align the power supply with the power supply slot.
4. Insert the power supply into the slot and press against the semicircular handle until you hear the power supply snap into place.

Figure 3. Insert the Replacement AC Power Supply



Figure 4. Insert the Replacement DC Power Supply



5. Connect the power supply to a power source. If connecting all power supplies, plug separate power cords into the power supplies and connect them to separate wall sockets.

Note

The Citrix ADC SDX appliance emits a high-pitched alert if the following conditions are met:

- One power supply fails.
- If you connect only one power cable to the appliance in which two power supplies are installed.

To silence the alarm, press the button labeled Alarm Disable on the back panel of the appliance. The **Disable alarm button** is functional only when the appliance has two power supplies.

Solid-State drives


In a Citrix ADC SDX appliance, the solid-state drives (SSD) store system bootup files and VDI of Management Service instances. Some support RAID and some do not.

SSDs with RAID support are hot swappable.

To replace a RAID-supported SSD**

1. From the Citrix ADC SDX GUI, navigate to **Configuration > System > RAID > Physical Drives**. Under **Raid State** you can identify the failed SSD.
2. Select the check box and click **Locate** to identify the failed SSD at the back panel. Click **Stop Locate** after you've identified the drive.
3. Next, click **Prepare to Remove**.
4. Click **Physical Drives**. The state of the drive must now appear as **Not Present**.
5. Locate the SSD on the back panel of the appliance. Push the safety latch of the drive cover down while pulling out on the drive handle to disengage. Pull out the faulty drive.


Figure 5. Remove an Existing SSD

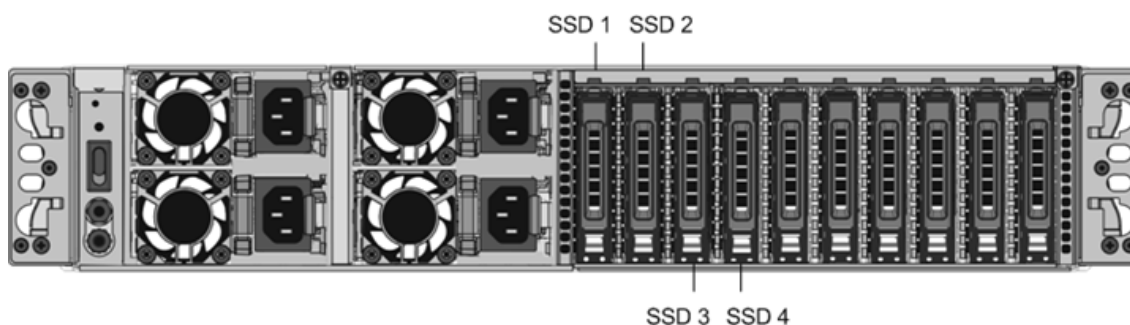

6. Verify that the replacement SSD is the correct size by comparing the replacement drive size with the removed drive. For example, if the removed drive is 480 GB, the replacement drive must also be 480 GB.
7. Open the drive handle fully up, and insert the new Citrix-certified SSD into the slot as far as possible. To seat the drive, close the handle flush with the rear of the appliance so that the drive locks securely into the slot.

When inserting the drive, orient the drive handle the same way as the installed drives.

Figure 6. Insert a Replacement SSD

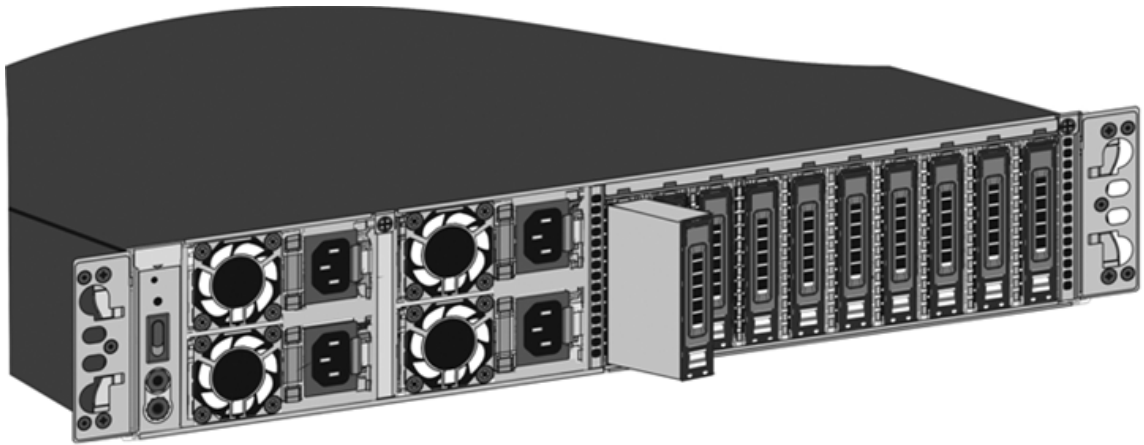


- In the Citrix ADC GUI, click the refresh icon for the list of physical drives. The state of the drive must appear as Present. After you replace one of the SSDs, the configuration on the other SSD in the mirrored SSD is copied to the replacement SSD.

To replace an SSD without RAID support

- From the Citrix ADC SDX GUI, navigate to **Configuration > System**, and in the System pane, click **Shutdown Appliance**.
- Locate the SSD on the back panel of the appliance.
- Press the latch release button, and the handle rotates out. Pull the handle to remove the drive.

Figure 7. Remove an Existing SSD without RAID

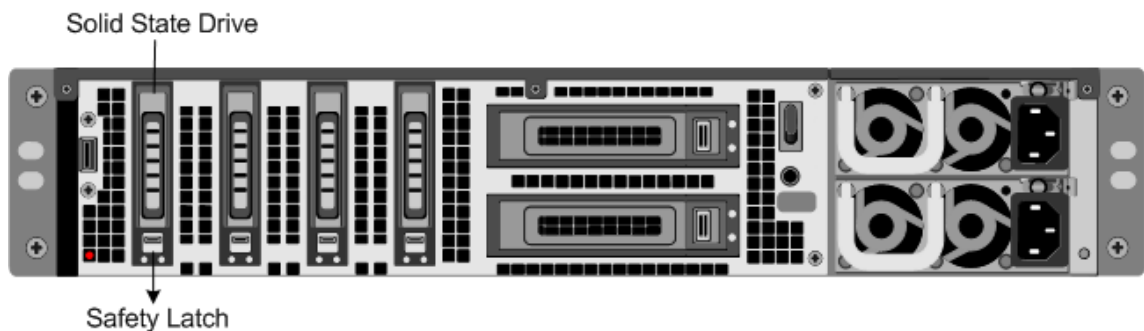

- Verify that the replacement SSD is the correct size by comparing the replacement drive size with the removed drive. For example, if the removed drive is 480 GB, the replacement drive must be 480 GB.
- Pick up the new SSD, open the drive handle fully to the left or up, and insert the drive into the slot as far as possible. To seat the drive, close the handle flush with the rear of the appliance so that the drive locks securely into the slot.

When inserting the drive, orient the drive handle the same way as the installed drives.

Figure 8. Insert a Replacement SSD without RAID

6. Turn on the appliance by manually pressing the power switch or by logging on to lights out management.
7. Log on to the default IP address by using a web browser, or connect to the serial console by using a console cable. Next, perform the initial configuration.
8. Upload a platform license and any optional feature licenses, including universal licenses, to the Citrix ADC appliance.
9. After the correct Citrix ADC software version is loaded, you can restore the working configuration.

Direct attach cable

A direct attach cable (DAC) assembly is a high performance integrated duplex data link for bi-directional communication. The cable is compliant with the IPF MSA (SFF-8432) for mechanical form factor and SFP+ MSA for DACs. The cable, which can be up to 5 meters long, is data-rate agnostic. Supporting speeds more than 10 Gbps, it is a cost-effective alternative to optical links (SFP+ transceivers and fiber optic cables.) The transceiver with DAC is hot-swappable. You can insert and remove the transceiver with the attached cable without shutting down the appliance. The Citrix ADC appliance supports only the passive DAC.

Points to note:

- DAC is supported only on 10G ports. Do not insert a DAC into a 1G port.
- Do not attempt to unplug the integrated copper cable from the transceiver and insert a fiber cable into the transceiver.


Note

Autonegotiation is not supported on an interface to which a DAC is connected.

To replace a DAC


1. To remove the DAC, pull the tab on the top of the DAC, and then pull the DAC out of the port.

Figure 9. Remove a DAC from the 10G port

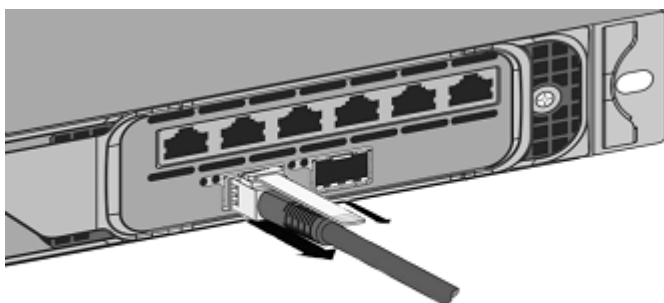

2. To insert the DAC, slide it into the 10G port on the appliance. You hear a click when the DAC properly fits into the port.

Figure 10. Insert a DAC into the 10G port

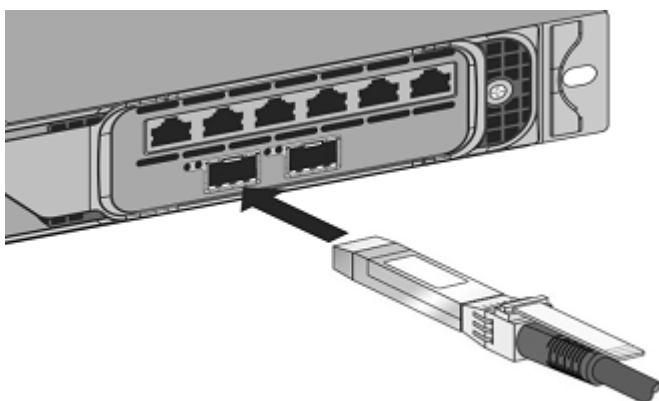

Safety, cautions, warnings, and other information

August 29, 2020

Read the safety and other compliance information before unpacking and installing the product. The safety and other compliance information remains the same for both SDX and MPX appliances. See the following documents:

- [Safety, cautions, warnings, and other information.](#)
- [Taiwan BSMI RoHS statement](#)

Note: For the list of safety certifications, standards, and ROHS compliance for each model, see the data sheet. The data sheet is available on www.citrix.com. Hover your mouse pointer on Products, and in the Networking list, select **Citrix ADC**.

- [FCC compliance statement](#)

Prepare for installation

August 29, 2020

Before you install your new appliance, carefully unpack your appliance and make sure that all parts were delivered. Verify that the location where the appliance is to be installed meets temperature and power requirements. Ensure that the server cabinet or floor-to-ceiling cabinet is securely bolted to the floor and has sufficient airflow.

Only trained and qualified personnel must install, maintain, or replace the appliance, and efforts must be taken to ensure that all cautions and warnings are followed.

This document includes the following details:

- Unpacking the appliance
- Preparing the site and rack
- Electrical safety precautions

Unpack the appliance

The hardware accessories for your particular appliance, such as cables, adapters, and rail kit, vary depending on the hardware platform you ordered. Unpack the box that contains your new appliance on a sturdy table with plenty of space and inspect the contents.

Use the following list to verify that you received everything that must have been included in the box.

- The appliance you ordered
 - One RJ-45 to DB-9 adapter
 - One 6 ft RJ-45/DB-9 cable
 - The following list specifies the number of power cables included for each appliance model:
 - One power cable for the SDX 8015/8400/8600 appliances
 - Two power cables for the SDX 11500/13500/14500/16500/18500/20500, SDX 11515/11520/11530/11540, and SDX 17500/19500/21500, and SDX 17550/19550/20550/21550 appliances
 - Four power cables for the SDX 22040/22060/22080/22100/22120 and SDX 24100/24150 appliances

Note: Make sure that a power outlet is available for each cable.

Note: For Brazilian customers, Citrix does not ship a power cable. Use a cable that conforms to the **ABNT NBR 14136:2002** standard.
 - One standard 4-post rail kit
- Note: If the kit that you received does not fit your rack, contact your Citrix sales representative to order the appropriate kit.

In addition to the items included in the box with your new appliance, you need the following items to complete the installation and initial configuration process.

- Ethernet cables for each additional Ethernet port that you connect to your network
 - One available Ethernet port on your network switch or hub for each Citrix ADC Ethernet port you want to connect to your network
- Note: Transceiver modules are sold separately. Contact your Citrix sales representative to order transceiver modules for your appliance. Only transceivers supplied by Citrix are supported on the appliance.
- A computer to serve as a management workstation

Prepare the site and rack

There are specific site and rack requirements for the Citrix ADC appliance. Ensure that adequate environmental control and power density are available. Racks must be bolted to the ground, have sufficient airflow, and have adequate power and network connections. Preparing the site and rack are important steps in the installation process and help ensure a smooth installation.

Site requirements

The appliance must be installed in a server room or server cabinet with the following features:

- **Environment control**

An air conditioner, preferably a dedicated computer room air conditioner (CRAC), capable of maintaining the cabinet or server room at a temperature of no more than 27 degrees C/80.6 degrees F at altitudes of up to 2100 m /7000 ft, or 18 degrees C/64.4 degrees F at higher altitudes, a humidity level no greater than 45 percent, and a dust-free environment.

- **Power density**

Wiring capable of handling at least 4000 watts per rack unit in addition to power needs for the CRAC.

Rack requirements

The rack on which you install your appliance must meet the following criteria:

- Rack characteristics

Racks must be either integrated into a purpose-designed server cabinet or be the floor-to-ceiling type, bolted down at both top and bottom to ensure stability. If you have a cabinet, it must be installed perpendicular to a load-bearing wall for stability and sufficient airflow. If you have a server room,

your racks must be installed in rows spaced at least 1 meter/3 ft apart for sufficient airflow. Your rack must allow your IT personnel unfettered access to the front and back of each server and to all power and network connections.

- Power connections

At minimum, two standard power outlets per unit.

- Network connections

At minimum, four Ethernet connections per rack unit.

- Space requirements

One empty rack unit for the Citrix ADC SDX 8015/8400/8600, and two consecutive empty rack units for all other appliance models.

You can order the following rail kits separately.

- Compact 4-post rail kit, which fits racks of 23–33 inches.
- 2-post rail kit, which fits 2-post racks.

Electrical safety precautions

Read the caution and danger information you need to know, before unpacking and installing the product. For more information, see [Safety, cautions, warnings, and other information](#).

Install the hardware

January 1, 2021

Determining that the location where you plan to install your appliance meets the environmental standards and the server rack is in place according to the instructions. After you mount the appliance, you are ready to connect it to the network, to a power source, and to the console terminal that you will use for initial configuration. To complete the installation, you turn on the appliance. Be sure to observe the cautions and warnings listed with the installation instructions.

Note: Keep the serial number handy before you rack-mount the appliance. The serial number is the password for the first time logon to the appliance and can be found at the back of the appliance.

Rack-mount the appliance

Most appliances can be installed in standard server racks that conform to the EIA-310-D specification. The appliances ship with a set of rails, which you must install before you mount the appliance. The

only tools that you need for installing an appliance are a Phillips screwdriver and a flathead screwdriver.

Caution: If you are installing the appliance as the only unit in the rack, mount it at the bottom. If the rack contains other units, make sure that the heaviest unit is at the bottom. If the rack has stabilizing devices available, install them before mounting the appliance.

To check the different hardware platforms and the rack units required for each platform, see the details given for each model under [SDX hardware platforms](#).

Each appliance ships with a mounting rail kit that contains two rail assemblies, one each for the left and the right side of the appliance, and screws to attach the rails. An assembly consists of an inner rail and a rack rail. The supplied rail kit is 28 inches long (38 inches extended). Contact your Citrix sales representative to order a 23 inches (33 inches extended) rail kit.

Note: The same rail kit is used for both square-hole and round-hole racks. See To install the rack rails on the rack for specific instructions for threaded, round-hole racks.

To mount the appliance, you must first install the rails and then install the appliance in the rack.

Perform the following tasks to mount the appliance:

- Remove the inner rails from the rail assembly.
- Attach the inner rails to the appliance.
- Install the rack rails on the rack.
- Install the appliance in the rack.

The appliance is shipped with rack-rail hardware. This hardware consists of two inner rails that you attach to the appliance, one on each side, and a rack-rail assembly that you attach to the rack. The following figure illustrates the steps involved in mounting the Citrix ADC SDX appliance to a rack.

Remove the inner rails from the rail assembly

1. Place the rail assembly on a flat surface.
2. Slide out the inner rail toward the front of the assembly.
3. Press the latch until the inner rail comes all the way out of the rail assembly.
4. Repeat steps 1 through 3 to remove the second inner rail.

Attach the inner rails to the appliance

1. Position the right inner rail behind the handle on the right side of the appliance.
2. Align the holes on the rail with the corresponding holes on the side of the appliance.

3. Attach the rail to the appliance with the provided screws: 4 per side for a 1U appliance and 5 per side for a 2U appliance, as shown in the following figure.

Figure 1. Attaching inner rails



4. Repeat steps 1 through 3 to install the left inner rail on the other side of the appliance.

Install the rack rails on the rack

1. If you have a round-hole, threaded rack, skip to step 3.
2. Install square nut retainers into the front post and back post of the rack as shown in the following figures. Before inserting a screw, be sure to align the square nut with the correct hole for your 1U or 2U appliance. The three holes are not evenly spaced.

Figure 2. Installing Retainers into the Front Rack Posts

Install in this hole for a 2U appliance

Install in center hole for a 1U appliance



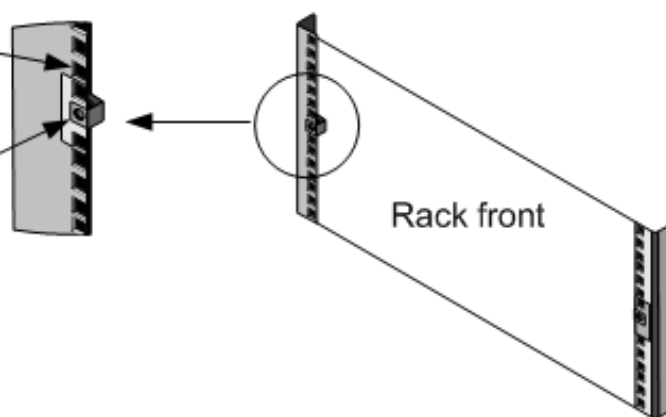


Figure 3. Installing Retainers into the Rear Rack Posts

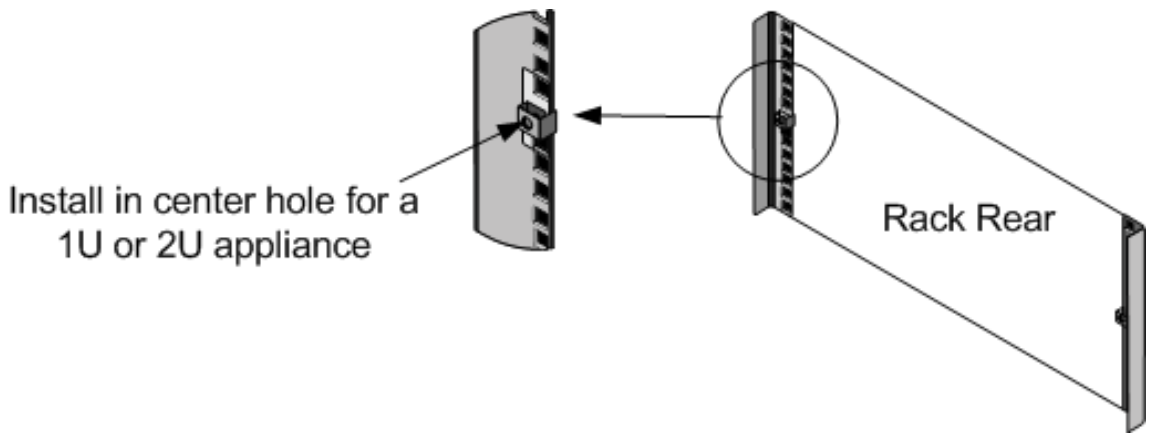

3. Install the adjustable rail assembly into the rack as shown in the following figures. Use a screw to lock the rear rail flange into the rack. With the screw securing the rail in place, you can optionally remove the latching spring.


Figure 4. Installing the Rail Assembly to the Rack

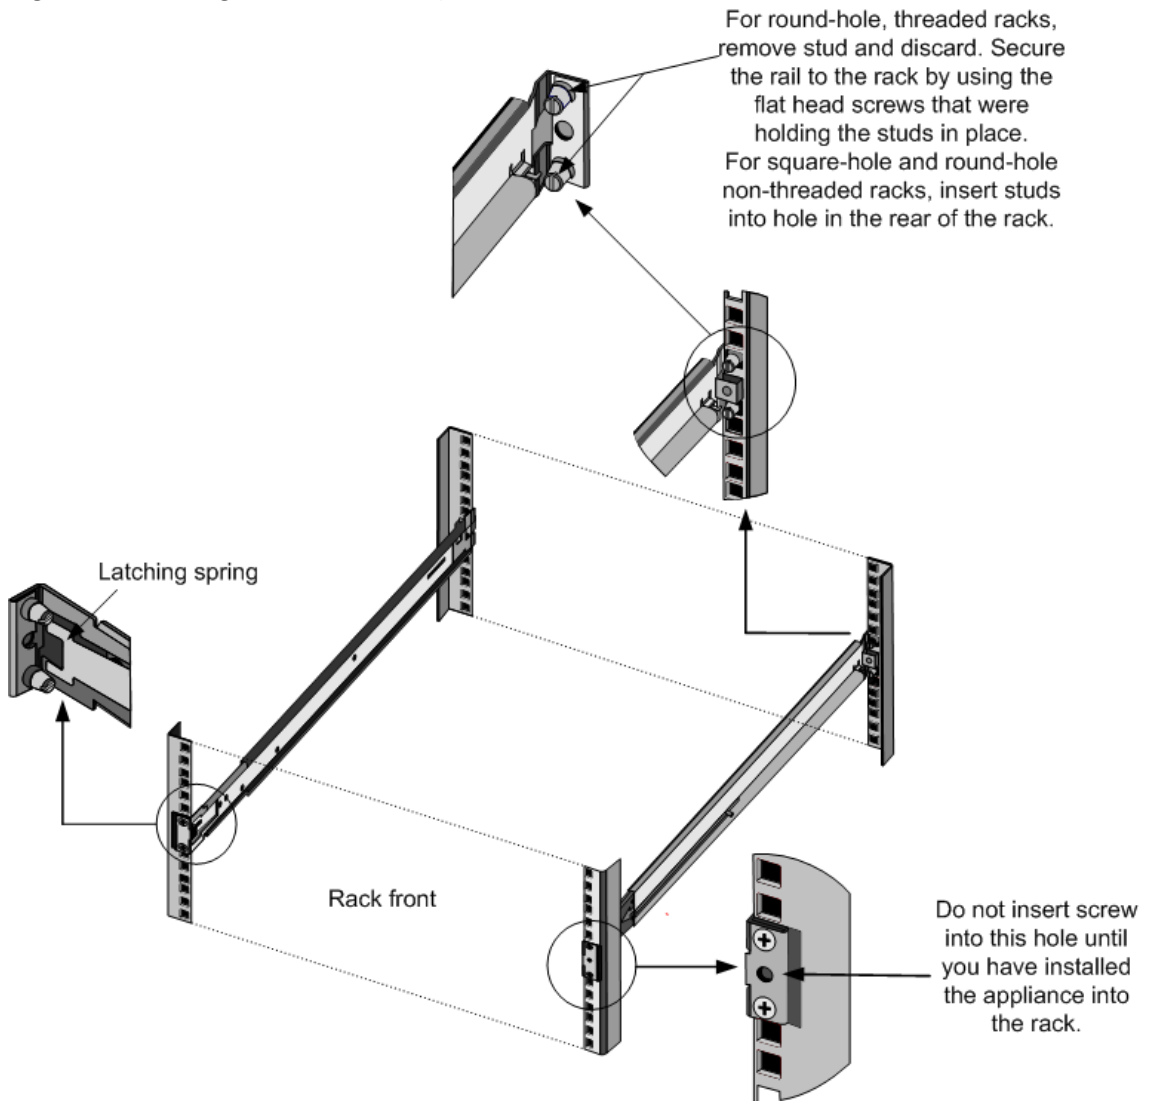

Install the appliance in the rack

1. Align the inner rails, attached to the appliance, with the rack rails.
2. Slide the appliance into the rack rails, keeping the pressure even on both sides.
3. Verify that the appliance is locked in place by pulling it all the way out from the rack.

Figure 5. Rack Mounting the Appliance

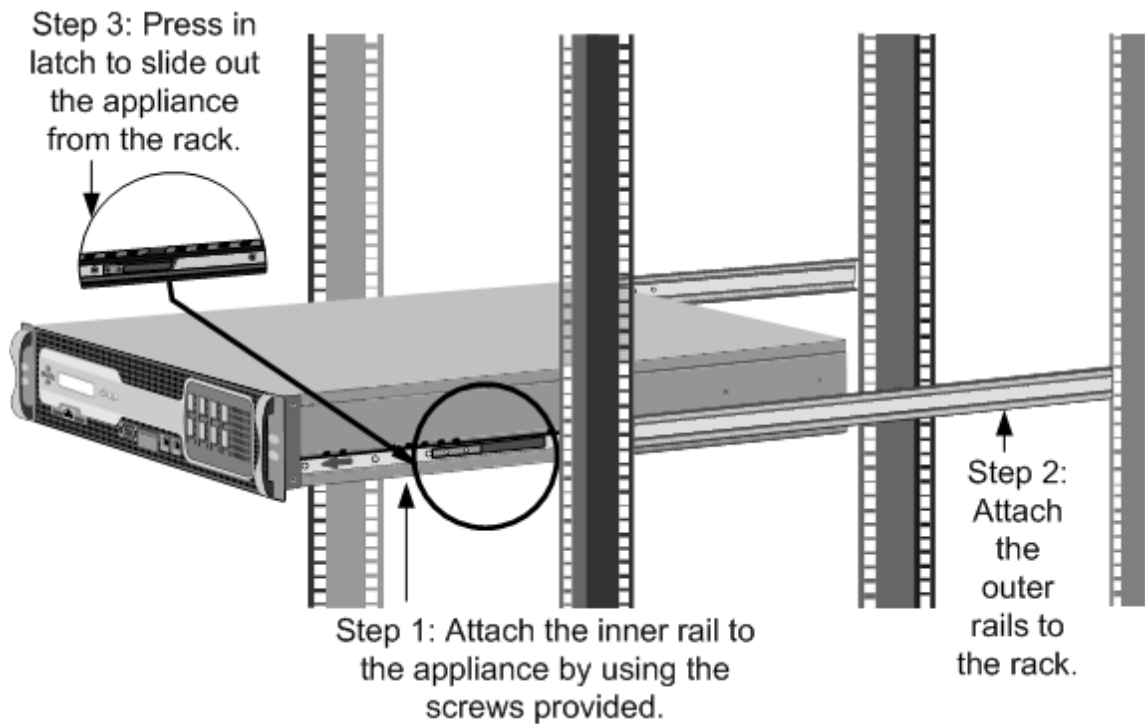

Watch this quick video about [how to rack mount a Citrix ADC hardware appliance](#).

Install and remove 1G SFP transceivers

A Small Form-Factor Pluggable (SFP) is a compact transceiver that can operate at speeds of up to 1 gigabit per second and is available in both copper and fiber types. Inserting a 1G SFP copper transceiver converts the 1G SFP port to a 1000BASE-T port. Inserting a 1G SFP fiber transceiver converts the 1G SFP port to a 1000BASE-X port. Auto-negotiation is enabled by default on the 1G SFP port into which you insert your 1G SFP transceiver. When a link between the port and the network is established, the speed and mode are matched on both ends of the cable.

Caution: Citrix ADC appliances do not support 1G SFP transceivers from vendors other than Citrix Systems. Attempting to install third-party 1G SFP transceivers on your Citrix ADC appliance voids the warranty.

Insert 1G SFP transceivers into the 1G SFP ports on the front panel of the appliance. Frequent installation and removal of transceivers shortens their life span. Follow the removal procedure carefully to

avoid damaging the 1G SFP transceiver or the appliance.

Caution: Do not install the transceivers with the cables attached. Doing so can damage the cable, the connector, or the optical interface of the transceiver.


Install a 1G SFP transceiver

1. Remove the 1G SFP transceiver carefully from its box.
Danger: Do not look directly into fiber optic transceivers or cables. They emit laser beams that can damage your eyes.
2. Align the 1G SFP transceiver to the front of the 1G SFP transceiver port on the front panel of the appliance, as shown in the following figure.

Note

The illustration in the following figures might not represent your actual appliance.

Figure 6. Installing a 1G SFP transceiver

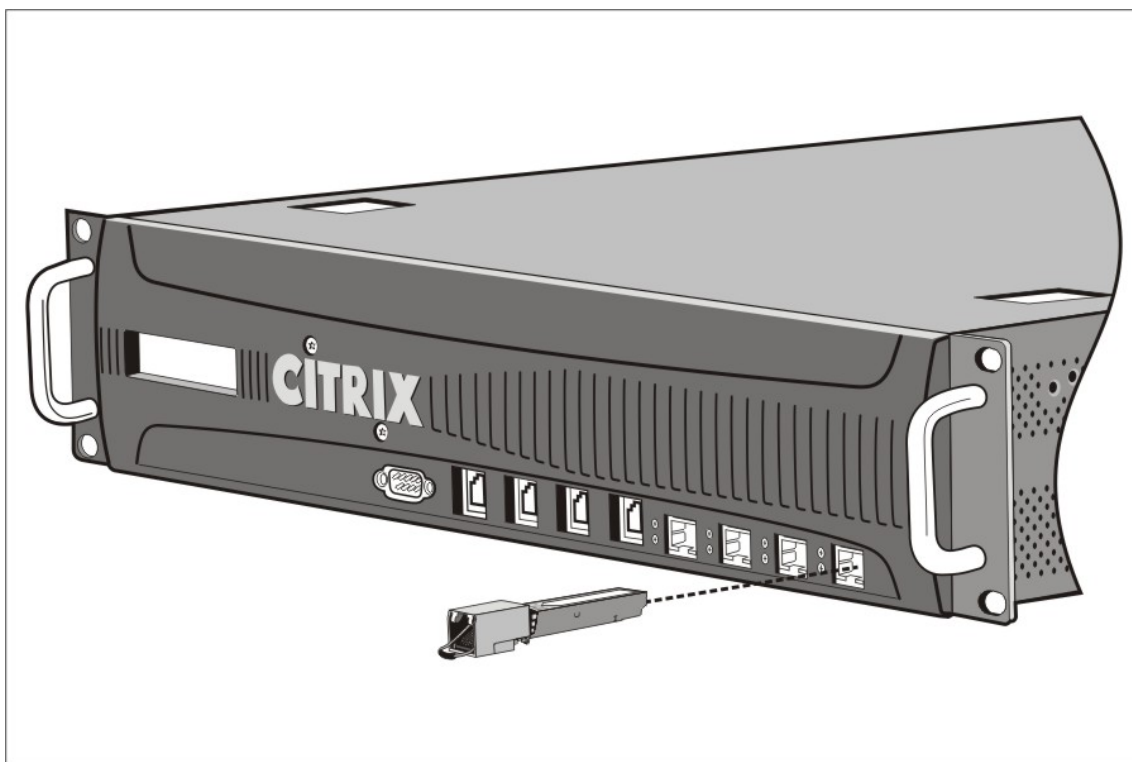

3. Hold the 1G SFP transceiver between your thumb and index finger and insert it into the 1G SFP transceiver port. Press it in until you hear the transceiver snap into place.
4. Lock the transceiver.
5. Verify that the LED is green and blinks twice, which indicates that the transceiver is functioning correctly.

6. When using a fiber 1G SFP transceiver, do not remove the dust caps attached to the transceiver and the cable until you are ready to insert the cable.

Remove a 1G SFP transceiver

1. Disconnect the cable from the 1G SFP transceiver. If you are using a fiber optic cable, replace the dust cap on the cable before putting it away.
Danger: Do not look directly into fiber optic transceivers or cables. They emit laser beams that can damage your eyes.
2. Unlock the 1G SFP transceiver.
3. Hold the 1G SFP transceiver between your thumb and index finger and slowly pull it out of the port.
4. If you are removing a fiber 1G SFP transceiver, replace the dust cap before putting it away.
5. Put the 1G SFP transceiver into its original box or another appropriate container.

Install and remove 10G SFP+ transceivers

A 10-Gigabit Small Form-Factor Pluggable (SFP+) is a compact optical transceiver that can operate at speeds of up to 10 gigabits per second. Autonegotiation is enabled by default on the 10G SFP+ ports into which you insert your 10G SFP+ transceiver. When a link between the port and the network is established, the mode is matched on both ends of the cable and for 10G SFP+ transceivers, the speed is also autonegotiated.

Caution: Citrix ADC appliances do not support 10G SFP+ transceivers provided by vendors other than Citrix Systems. Attempting to install third-party 10G SFP+ transceivers on your Citrix ADC appliance voids the warranty.

Insert the 10G SFP+ transceivers into the 10G SFP+ ports on the front panel of the appliance. Frequent installation and removal of transceivers shortens their life span. Follow the removal procedure carefully to avoid damaging the transceiver or the appliance.

Caution: Do not install the transceivers with the cables attached. Doing so can damage the cable, the connector, or the optical interface of the transceiver.

Install a 10G SFP+ transceiver

1. Remove the 10G SFP+ transceiver carefully from its box.
Warning: Do not look directly into fiber optic transceivers and cables. They emit laser beams that can damage your eyes.
2. Align the 10G SFP+ transceiver to the front of the 10G SFP+ transceiver port on the front panel of the appliance.

3. Hold the 10G SFP+ transceiver between your thumb and index finger and insert it into the 10G SFP+ transceiver port, pressing it in until you hear the transceiver snap into place.
4. Move the locking hinge to the DOWN position.
5. Verify that the LED is green and blinks twice, which indicates that the transceiver is functioning correctly.
6. Do not remove the dust caps attached to the transceiver and cable until you are ready to insert the cable.

Remove a 10G SFP+ transceiver

1. Disconnect the cable from the 10G SFP+ transceiver. Replace the dust cap on the cable before putting it away.
Danger: Do not look directly into fiber optic transceivers or cables. They emit laser beams that can damage your eyes.
2. Unlock the 10G SFP+ transceiver by moving the locking hinge to the UP position.
3. Hold the 10G SFP+ transceiver between your thumb and index finger and slowly pull it out of the port.
4. Replace the dust cap on the transceiver before putting it away.
5. Put the 10G SFP+ transceiver into its original box or another appropriate container.

Connect the cables

When the appliance is securely mounted on the rack, you are ready to connect the cables. Ethernet cables and the optional console cable are connected first. Connect the power cable last.

Warning: Before installing or repairing the appliance, remove all jewelry and other metal objects that might come in contact with power sources or wires. When you touch both a live power source or wire and ground, any metal objects can heat up rapidly and cause burns, set clothing on fire, or fuse the metal object to an exposed terminal.

Connect the Ethernet cables

Ethernet cables connect your appliance to the network. The type of cable you need depends on the type of port used to connect to the network. Use a category 5e or category 6 Ethernet cable with a standard RJ-45 connector on a 10/100/1000BASE-T port or 1G SFP copper transceiver. Use a fiber optic cable with an LC duplex connector with a 1G SFP fiber transceiver, 10G SFP+ transceiver. The type of connector at the other end of the fiber optic cable depends on the port of the device that you are connecting to.

Connect an Ethernet cable to a 10/100/1000BASE-T port or 1G SFP copper transceiver

1. Insert the RJ-45 connector on one end of your Ethernet cable into an appropriate port on the front panel of the appliance, as shown in the following figure.

Figure 7. Inserting an Ethernet cable



2. Insert the RJ-45 connector on the other end into the target device, such as a router or switch.
3. Verify that the LED glows amber when the connection is established.

Connect the Ethernet cable to a 1G SFP fiber, 10G SFP+ transceiver

1. Remove the dust caps from the transceiver and cable.
2. Insert the LC connector on one end of the fiber optic cable into the appropriate port on the front panel of the appliance.
3. Insert the connector on the other end into the target device, such as a router or switch.
4. Verify that the LED glows amber when the connection is established.

Connect the Console cable


You can use the console cable to connect your appliance to a computer or terminal, from which you can configure the appliance.

Alternatively, you can use a computer connected to the network. Before connecting the console cable, configure the computer or terminal to support VT100 terminal emulation, 9600 baud, 8 data bits, 1 stop bit, parity, and flow control set to NONE. Then connect one end of the console cable to the RS232 serial port on the appliance and the other end to the computer or terminal.

Connect the console cable to a computer or terminal

1. Insert the DB-9 connector at the end of the cable into the console port that is located on the front panel of the appliance, as shown in the following figure.

Figure 8. Inserting a console cable

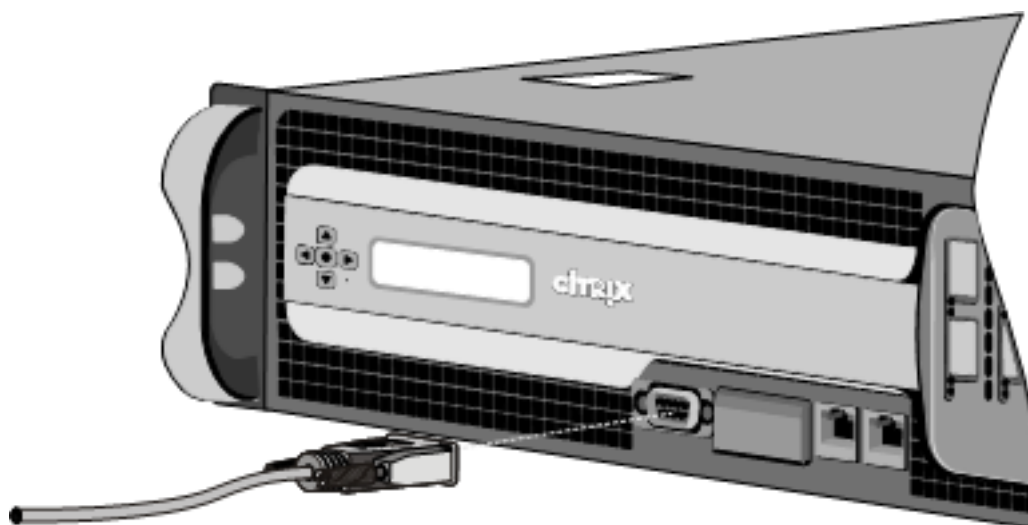

Note

To use a cable with an RJ-45 converter, insert the optional converter provided into the console port and attach the cable to it.

2. Insert the RJ-45 connector at the other end of the cable into the serial port of the computer or terminal.


Connect the power cable

An SDX 8015/8400/8600 appliance has one power cable. All the other appliances come with two power cables, but they can also operate if only one power cable is connected. A separate ground cable is not required, because the three-prong plug provides grounding.

Connect the appliance to the power source

1. Connect one end of the power cable to the power outlet on the back panel of the appliance, next to the power supply, as shown in the following figure.

Figure 9. Inserting a power cable

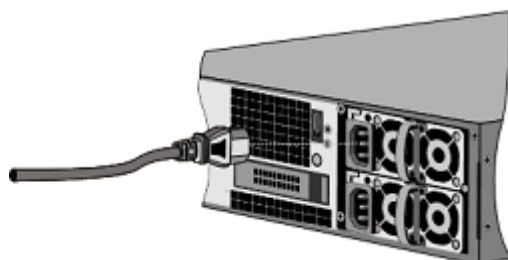

2. Connect the other end of the power cable to a standard 110V/220V power outlet.
3. If a second power supply is provided, repeat steps 1 and 2 to connect the second power supply.

Note

The SDX 11500/13500/14500/16500/18500/20500, SDX 11515/11520/11530/11540/11542, SDX 17500/19500/21500, and SDX 17550/19550/20550/21550 appliances emit a high-pitched alert if one power supply fails or if you connect only one power cable to the appliance. To silence the alarm, you can press the small red button located on the back panel of the appliance.

Switch on the appliance

After you have installed the appliance in a rack and connected the cables, verify that the power cable is properly connected. If you have installed a second power supply, make sure the second cable is connected to an outlet for a different circuit than the first. After verifying the connections, you are ready to switch on the appliance.

To switch on the appliance

1. Verify that the appliance is connected through a console or Ethernet port. This check ensures that you can configure the appliance after it is switched on.
2. Press the ON/OFF toggle power switch on the back panel of the appliance.

Caution: Be aware of the location of the emergency power off (EPO) switch, so that if an electrical accident occurs you can quickly remove power from the appliance.

Initial configuration

August 27, 2021

After you have installed your appliance in a rack, you are ready to perform the initial configuration. To perform the initial configuration, you can use the Management Service user interface or the serial console. You can access the Management Service user interface from any computer that is on the same network as the new SDX appliance. If you do not have a computer on the same network, use the serial console to perform the initial configuration of the SDX appliance. Citrix recommends that, when you complete the initial configuration, you change the root-user password. For information about changing the root-user password, see [Configuring Authentication and Authorization Settings](#).

Determine the following information for performing the initial configuration.

- Citrix ADC SDX IP address and subnet mask: The management IP address and the mask used to define the subnet in which the SDX appliance is located. This IP address is used to access the Citrix ADC SDX Management Service user interface.

- Citrix Hypervisor IP address: The IP address of the Citrix Hypervisor.
- Default gateway: The IP address of the router that forwards traffic out of the appliance's subnet. The default gateway must be in the same subnet as the NSIP address.
- Root password: The root user has full administrative privileges on the appliance. The root password is used to authenticate the root user. Change this password during the initial configuration of the appliance.

This topic includes the following sections:

- Initial Configuration through the Management Service User Interface
- Initial Configuration through the Serial Console
- Changing the Password of the Default User Account

Initial configuration through the Management Service user interface

To set up the appliance by using the Management Service user interface, connect a workstation or laptop to the same network as the appliance.

To configure the Citrix ADC SDX appliance by using the Management Service user interface

1. Connect the Citrix ADC SDX appliance to a management workstation or network by using interface 0/1.
2. Open a browser and type: <http://192.168.100.1>

Note: The Citrix ADC SDX Management Service is preconfigured with the IP address 192.168.100.1 and the Citrix Hypervisor is preconfigured with the IP address 192.168.100.2.

1. In **User Name**, type `nsroot`. In **Password**, if the earlier default password does not work, try typing the serial number of the appliance. The serial number bar code is available at the back of the appliance. Citrix recommends that you change the password after the first logon. For information about changing the password, see [Change the administrative password](#).
2. In the navigation pane, click **System**.
3. In the details pane, under **Setup Appliance**, click **Network Configuration**.
4. In the **Network Configuration** page, do the following:

← Network Configuration

Interface*

Appliance supportability IP*

Gateway*

DNS

IPv4

Appliance Management IP*

Netmask*

IPv6

Management Service IPv6 Address*

Gateway IPv6 Address*

Additional DNS

×

×

OK

Close

a. In the **Interface** field, select the management interface that connects the appliance to a management workstation or network. Possible values: 0/1, 0/2. Default: 0/1.

Note: If you create an LA channel of the management ports, you can assign only one IP address to the channel. In the **Interface** field, only the LA channel option appears instead of 0/1 and 0/2. Also, even if both ports are connected, the Management Service is active only on one port.

b. In the **Appliance supportability IP** field, enter the IP address of the Citrix Hypervisor.

c. In the **Gateway** field, enter the IP address of the router that forwards traffic out of the appliance's subnet.

d. In the **DNS** field, enter the IPv4 address of the primary DNS server.

Note: IPv6 addresses are not support for the primary DNS server.

e. Select the IPv4 check box if you want to use the IPv4 address for the Management Service and enter the details for the following parameters:

i. **Appliance Management IP** — The IPv4 address that is used to access the Management Service by using a Web browser.

ii. **Netmask** —The mask used to define the subnet in which the SDX appliance is located.

f. Select the **IPv6** check box if you want to use the IPv6 address for the Management Service and enter the details for the following parameters:

i. **Management Service IP Address** —The IPv6 address that is used to access the Management Service by using a Web browser.

Note

The Citrix Hypervisor IP address and Management Service IP address must be in the same subnet.

ii. **Gateway IPv6 Address** — The IPv4 address of the router that forwards traffic out of the appliance's subnet.

g. Select the **Additional DNS checkbox** to add DNS server IP addresses as an extra DNS server apart from the primary DNS server. The IP addresses can be either IPv4 or IPv6.

Note:

Make sure that:

- You add a DNS server IP address or two DNS server IP address as an extra DNS server.
- You do not use the same DNS server IP address for the primary DNS server and extra DNS servers.
- Cascading of DNS servers for authentication, authorization, and auditing is not supported. For authentication, authorization, and auditing of LDAP referrals, RADIUS, and TACACS, the primary DNS server configured for address resolution is always considered for authentica-

tion, authorization, and auditing.

8. Click **OK**, and then click **Close**.

To confirm that the appliance is configured correctly, ping the new Management Service IP address or use the new IP address to open the user interface in a browser.

Note:

Log on to the Citrix ADC SDX appliance using the CLI, make sure that the file `/etc/resolv.conf` file included the added extra DNS server IP addresses. Also, the `/mpsconfig/svm.conf` file reflects the added extra DNS server IP addresses.

For example:

```
1 /mps/changenameserver.sh 127.0.0.1
2 /mps/addnameserver.sh 1.2.3.4
3 <!--NeedCopy-->
```

Initial Configuration through the serial console

To perform the initial configuration of the SDX appliance from outside the L2 domain, connect to the console port of the appliance and follow the instructions carefully.

Note

The `networkconfig` utility is available from build 72.5 and later.

To configure the Citrix ADC SDX appliance by using the serial console

1. Connect the console cable into your appliance.
2. Connect the other end of the cable to your computer and run the vt100 terminal emulation program of your choice.
 - For Microsoft Windows, you can use HyperTerminal.
 - For Apple Macintosh OSX, you can use the GUI-based Terminal program or the shell-based telnet client.

Note: OSX is based on the FreeBSD UNIX platform. Most standard UNIX shell programs are available from the OSX command line.
 - To For UNIX-based workstations, you can use any supported terminal emulation program.
3. Press ENTER. The terminal screen displays the Logon prompt.

Note: You might have to press ENTER two or three times, depending on which terminal program you are using.
4. At the prompt, type: `ssh nsroot@169.254.0.10` to log on to the Management Service. In **Password**, if the earlier default password does not work, try typing the serial number of the appli-

ance. The serial number bar code is available at the back of the appliance. Citrix recommends that you change the password after the first logon. For information about changing the password, see [Change the administrative password](#).

5. Type `shell` to switch to the shell prompt and type `networkconfig`

You can now use the new IP address to log on to the Management Service user interface.

Change the password of the default user account

The default user account provides complete access to all features of the Citrix ADC SDX appliance. For security reasons, the administrator account must be used only when necessary, and only individuals whose duties require full access must know the password for the administrator account. Citrix recommends changing the administrator password frequently. If you lose the password, you can reset the password to the default by reverting the appliance settings to factory defaults, and you can then change the password.

You can change the password of the default user account in the **Users** pane. In the **Users** pane, you can view the following details:

- Name
 - Lists the user accounts configured on the SDX appliance.
- Permission
 - Displays the permission level assigned to the user account.

Change the administrative password by using the GUI

1. Log on to the appliance by using the administrative credentials.
2. Navigate to **System > User Administration > Users**.
3. In the **Users** pane, click the default user account, and then click **Modify**.
4. In the **Modify System User** dialog box, in **Password** and **Confirm Password**, enter the password of your choice.
5. Click **OK**.

For more information about more Citrix ADC SDX software configuration, see [Citrix ADC SDX software documentation](#).

Lights out management port of the Citrix ADC SDX appliance

May 20, 2021

The SDX ADC appliances have an Intelligent Platform Management Interface (IPMI), also known as the lights out management (LOM) port, on the front panel of the appliance. You can use the LOM port to remotely monitor and manage the appliance, independently of the Citrix ADC software.

By connecting the LOM port to a dedicated channel that is separate from the data channel, you can make sure that connectivity to the appliance is maintained even if the data network is down. Further you can reduce the data cable and data network as a single point of failure.

You can access the LOM port through a browser and use the GUI for most tasks. All tasks can be performed through the Citrix ADC shell.

You can use either the GUI or a shell for the following tasks:

- Configuring the network settings
- Health monitoring
- Power control operations
- Factory reset

Different Citrix appliances support different shells:

- For Citrix Hypervisor based Citrix ADC SDX appliances, use the dom0 Linux root shell. To access the dom0 shell, log on to the Citrix Hypervisor management IP address instead of the SDX Management Service IP address, using the `root` account, not the `nsroot` account.
- For Linux based appliances, use the Linux bash root shell.

Note

The terms LOM and Baseboard Management Controller (BMC) are used interchangeably.

Caution: LOM firmware versions are platform specific. Upgrading to a LOM firmware version other than the one shown for your platform in the LOM support matrix table, might result in the LOM becoming unusable.

LOM support matrix

The LOM support matrix shows the recommended LOM firmware version for different platforms.

Table. LOM support matrix

Hardware	Recommended Version
SDX 5900	4.58
SDX 8015	3.21
SDX 8900	4.61
SDX 11500	3.39

Hardware	Recommended Version
SDX 11500 NEBS	3.39
SDX 11515	3.39
SDX 14000	4.08
SDX 14000-40S	4.08
SDX 14000 FIPS	4.08
SDX 14000-40G	4.08
SDX 15000	5.56
SDX 15000-50G	5.56
SDX 17500	3.39
SDX 17550	3.39
SDX 22000	3.24
SDX 24000	4.08
SDX 25000A	4.08
SDX 25000TA	4.08
SDX 25000-40G	4.08
SDX 26000	5.56
SDX 26000-50S	5.56
SDX 26000-100G	5.56

Configure the network settings on the LOM port

March 9, 2021

The default IP address for initial access to the LOM port is 192.168.1.3. Change the default credentials and IP address the first time you log on. All LOM GUI operations require you to connect to the appliance by typing the LOM IP address in a web browser and then entering the administrator credentials. Alternatively, you can access LOM functionality through the command line by using the `ipmitool` utility. Using the `ipmitool` utility remotely, you can determine the LOM firmware version number, perform warm and cold restarts, configure LOM network settings, monitor the health of the appliance, and perform power control operations. The utility is available for download at <http://ipmitool.sourceforge.net/>. The `ipmitool` utility is also included in Citrix ADC MPX and CloudBridge/SDX (dom0) appliances

for initial LOM port network configuration. When using the shell, you can choose to use DHCP or static IP settings for initial network configuration. After configuring the network settings, you can use the `ipmitool` commands over the network. For example, the BMC firmware revision command would need the same user name, password, and IP address that is used to access the BMC/LOM GUI port.

For initial configuration, connect the network port on your laptop or workstation directly to the LOM port with a crossover cable, or to a switch in the same local subnet(192.168.1.x) as the LOM port. Assign a network-reachable IP address and change the default credentials. After saving the new settings, the LOM restarts and the changes take effect. After the restart, you must use the new address to access the LOM.

If you make a mistake that results in losing network connectivity at both the old and new IP addresses, you must use the local shell method to recover.

See the [Secure Deployment Guide](#) for best practices for managing administrative credentials and configuring your network for a secure LOM deployment.

Note

On all SDX platforms, except SDX 22040/22060/22080/22100/22120 and SDX 24100/24150, the LEDs on the LOM port are non-operational by design.

Tip: For first-time setup in a network, to facilitate troubleshooting, make sure that a laptop/PC is connected directly to the LOM port. If you can ping and access the LOM GUI at the default IP address (192.168.1.3) by using static addressing on the computer, but remote access does not work:

- Take a closer look at the network firewall settings and access control list (ACL) policies of all network devices along the network path.

Tip: If some LOM GUI features work but others do not (for example, normal Citrix ADC console output is visible in the Citrix ADC console window in the LOM GUI, but typing in the console does not work), try the preceding method to isolate the cause to the specific BMC protocol being blocked by the network.

Tip: Use the iKVM (HTML5) feature to access the LOM GUI. Alternately, use Java. Ensure that the latest Java updates are installed on your computer.

To configure the Citrix ADC LOM port by using the GUI

1. In a web browser, type <http://192.168.1.3> and enter the default user credentials.

Note

The Citrix ADC LOM port is preconfigured with IP address 192.168.1.3 and subnet mask 255.255.255.0.

2. On the **Configuration** tab, click **Network** and type new values for the following parameters:

- IP Address—IP address of the LOM port
 - Subnet Mask—Subnet mask used to define the subnet of the LOM port
 - Default Gateway—IP address of the router that connects the LOM port to the network.
3. Click **Save**.
 4. If you want to change the user credentials, navigate to **Configuration > Users**, select the user, click **Modify User**, and change the credentials.

To configure the Citrix ADC LOM port by using the shell

Note: You need superuser (admin) credentials to access the shell.

1. Configure the IP addressing mode:
 - To use DHCP, at the shell prompt, type:

```
ipmitool lan set 1 ipsrc dhcp
```

No further IP-level configuration is required.

- To use static addressing, at the shell prompt type:

```
1 >ipmitool lan set 1 ipsrc static
2 >ipmitool lan set 1 ipaddr (LOM IP address)
3 >ipmitool lan set 1 netmask (netmask IP address)
4 >ipmitool lan set 1 defgw ipaddr <default gateway IP address>
5 <!--NeedCopy-->
```

The BMC reboots to apply the changes. Pings to the BMC succeed after approximately 60 seconds.

2. Optionally, to configure Ethernet VLAN ID and priority, at the Citrix ADC shell prompt type:

```
1 >ipmitool lan set 1 vlan id <off|ID>
2 >ipmitool lan set 1 vlan priority <priority>
3 <!--NeedCopy-->
```

You can either disable or enable the VLAN. Set the VLAN ID to a value from 1 to 4094, and the VLAN priority to a value from 0 to 7. After the network settings have been correctly applied, you can access the `ipmitool` remotely from a physically separate machine over the network. For remote access, enter the BMC user name, BMC password, and the BMC IP address. For example, to run the `ipmitool mc info` command, at the shell prompt on a remote machine, type:

```
ipmitool -U <username> -P <password> -H <bmc IP address> mc info
```

Obtain health monitoring information

There are two Citrix ADC MIBs: the Citrix ADC software management MIB and the Citrix ADC IPMI LOM hardware management MIB. The software management MIB is primarily used for monitoring the application software and the application software's utilization of hardware resources, such as CPU % and memory %. It provides a high level view of the appliance and is therefore suitable for the application monitoring function carried out by an application group within an organization. The LOM MIB is used for monitoring the hardware health and therefore provides a lower level view of the appliance. This type of monitoring is more applicable to the network monitoring function carried out by a network monitoring group.

The LOM SNMP traps in the LOM MIB report hardware failures. The Citrix ADC SNMP traps in the Citrix ADC MIB report software failures and hardware load issues.

The Citrix ADC MIB has a small subset of hardware sensors. It does not cover any BIOS level failures, because the BIOS checks the hardware primarily during boot time, before the Citrix ADC software starts. If the BIOS detects a failure, it does not load the boot loader. If the boot loader does not load, the operating system does not load, and therefore the Citrix ADC SNMP software service responsible for sending the traps does not load.

The Citrix ADC software Management MIB issues a warning under the following conditions only:

1. If the failure is gradual enough for the main CPU to issue an SNMP alert. An electrical failure close to the CPU, such as a failed electrical capacitor, occurs too quickly for the CPU to issue an alert.
2. If the failure happens after the BIOS, Operating System, and SNMP service have started and normal boot-up has been successful.
3. If the failure happens while the operating system and other system software are in a stable enough state for the SNMP software service to run.

Whenever the Citrix ADC MIB is unable to report these warnings, because of hardware or software failure, the LOM MIB monitors and reports the warnings. The LOM microcontroller operates independently of the Citrix ADC software. To monitor the hardware and software of the Citrix ADC appliance, you must use both the Citrix ADC MIB and the LOM MIB.

The Citrix ADC IPMI LOM hardware management MIB SNMP firmware runs on the BMC microcontroller chip. The BMC chip CPU sends a warning in the case of a hardware failure, regardless of whether any of the preceding conditions occur. For example, if the BIOS halts the system during boot-up because of a memory DIMM failure, the BMC chip uses the BIOS POST code snooping mechanism to detect the failure, and sends a bad DIMM SNMP alert.

You can log on to the LOM port to view the health information about the appliance. All system sensor information, such as system temperature, CPU temperature, and status of fans and power supplies, appears on the sensor readings page. The Event Log records time stamps of routine events such as a power cycle, in addition to recording hardware-failure events. If SNMP traps are enabled, these events

can be sent to your SNMP Network Monitoring software. For more information about how to set up an SNMP alert, see [Configuring SNMP Alerts](#).

To obtain health monitoring information

1. In the **Menu** bar, click **System Health**.
2. Under **Options**, click **Sensor Readings**.

Install the MIB

Download the IPMI SNMP management information base (MIB) for your LOM firmware version, and import it into the SNMP monitoring software.

For a sample configuration, see <http://www.net-snmp.org/tutorial/tutorial-5/commands/snmptrap.html>. For the exact steps of this procedure specific to your environment, contact your SNMP network monitoring software provider.

Configure SNMP Alerts

You can configure SNMP alerts on the LOM. Optionally, you can configure an alert to send emails.

To configure the alerts, you can use the LOM GUI or the Citrix ADC shell.

To configure SNMP alerts on the LOM by using the GUI

1. Download the IPMI View utility from <ftp://ftp.supermicro.com/utility/IPMIView/> and install it on your computer. Use this utility to test the configuration. For more information, see the section about configuring the alert settings in the IPMI View User Guide at <http://supermicro.com>.
2. Open the IPMI View utility.
3. In the LOM GUI, navigate to **Configuration > Alerts**, click **Alert No 1**, and then click **Modify**.
4. Select the severity level of the events for which to generate alerts.
5. Set Destination IP to the IP address at which you installed the IPMI View utility.
6. Optionally, to receive alerts by email, specify an email address. To avoid receiving email for routine alerts, specify a severity higher than Informational.
7. Click **Save**.
8. The LOM starts sending alerts to the IPMI View utility within a minute or two. After the IPMI View utility starts receiving alerts from the LOM, reconfigure the destination IP address to point to your SNMP Network Management Software, such as HP OpenView.

Set up SNMP alerts on the LOM by using the Citrix ADC shell

To customize your filter and policy settings, see the IPMI Specification 2.0 rev. 1.1 documentation.

The latest IPMI specifications are available from the IPMI section of the Intel website:

<http://www.intel.com/content/www/us/en/servers/ipmi/ipmi-specifications.html>

Usually, customization in the SNMP Network Management Software is the preferred method, because it can be done one time at a central location. Therefore, the following settings send all events for all sensors to the SNMP network management software. These events are low traffic events and therefore do not result in any significant network usage.

To set up SNMP filters to allow all events:

```
ipmitool raw 4 0x12 0x6 0x10 0x80 1 1 0 0xff 0xff 0xff 0xff 0xff 0xff 0xff  
0 0xff 0 0 0xff 0 0 0xff 0
```

To set up a policy list for all sensors and events:

```
ipmitool raw 4 0x12 9 0x10 0x18 0x11 0x81
```

To set up a destination IP address for an SNMP event:

```
ipmitool lan alert set 1 1 ipaddr <x.x.x.x>
```

Where, is the IP address to which the SNMP event must be sent.

To specify an SNMP community string name:

```
ipmitool lan set 1 snmp <community string>
```

Installing a certificate and key on the LOM GUI

August 18, 2020

Citrix recommends using HTTPS to access the LOM GUI. To use HTTPS, you must replace the default SSL certificate with one from a trusted certificate authority and upload a private key to the LOM GUI.

To encrypt SNMP alerts, set up an SSL certificate and private key. In the GUI, navigate to **Configuration > SSL Certification** and apply the SSL certificate and private key. See the Citrix ADC Secure Deployment Guide for more information about how to securely deploy the LOM in your network. To enable encryption and learn the security measures for LOM, see <http://support.citrix.com/article/CTX129514>.


If you make a mistake, you must restore the [BMC to the factory defaults](#) to erase the certificate and key.

Note


The certificate file must contain only the certificate. The certificate and key must not be in the same file. Make sure that the certificate contains only the certificate and that the key file contains only the key.

To upload a trusted certificate and private key by using the LOM GUI


1. Navigate to **Configuration > SSL Certification**.

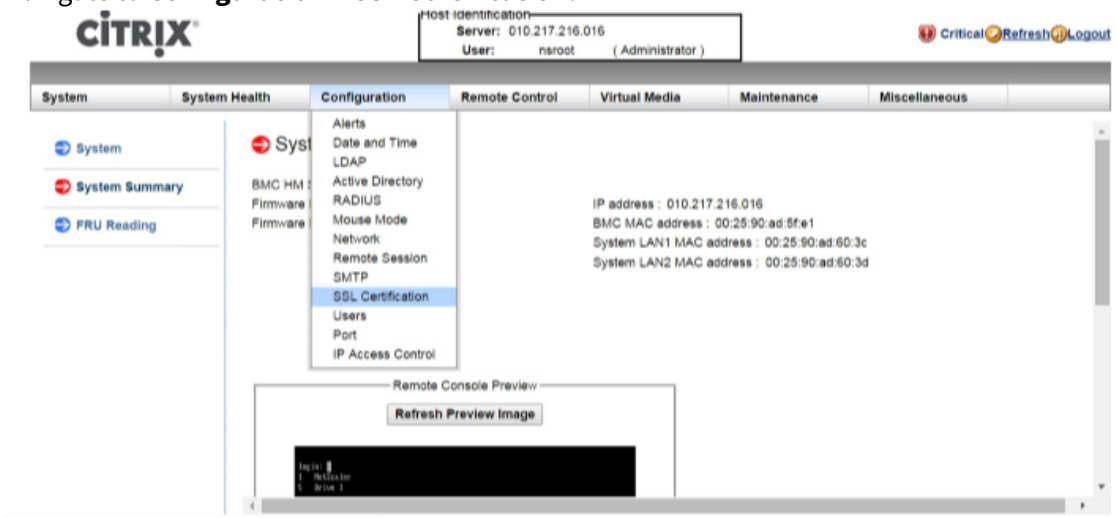


2. In the right pane, click the **Choose File** buttons to select a new SSL certificate and a new private key.

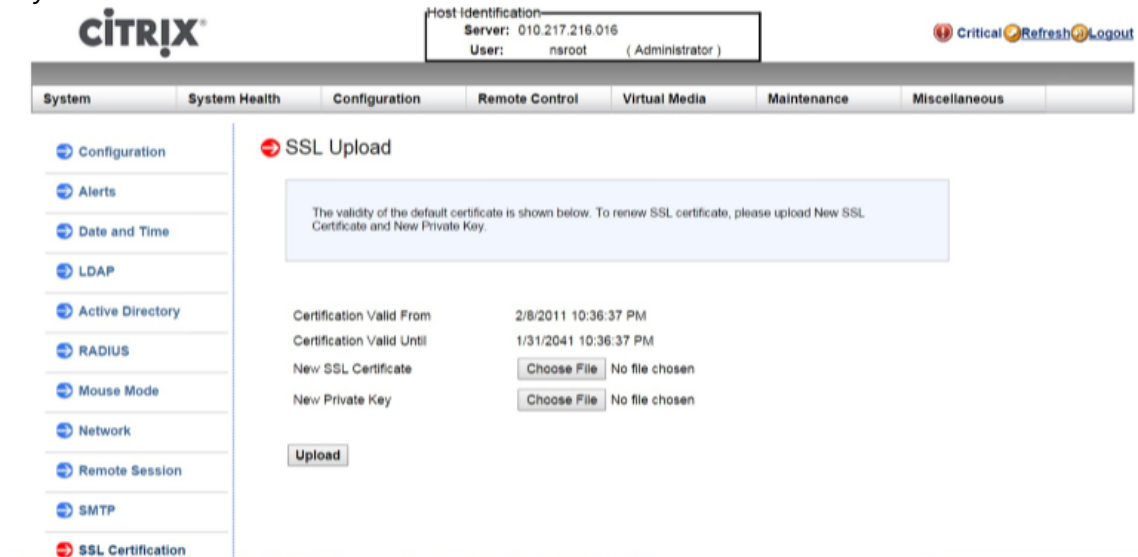


3. To verify that you have selected the correct certificate and private key, check the file names of the certificate and key. The file names appear next to the **Choose File** buttons.

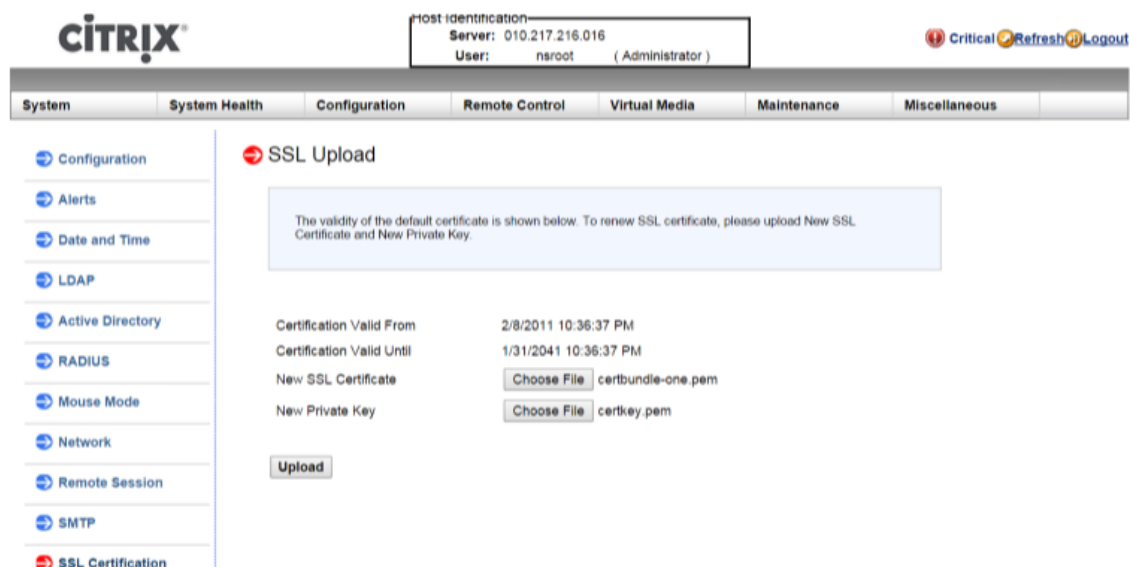


4. Click **Upload**. A message informs you that uploading a new SSL certificate replaces the existing (default) certificate.
5. Click **OK**.

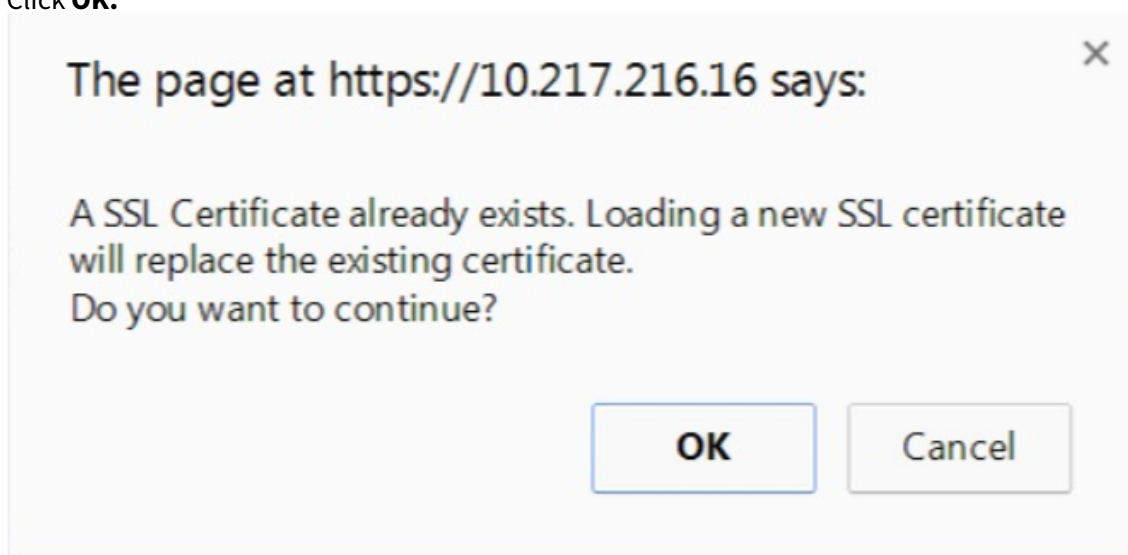

6. When a message informs you that the certificate and key have been uploaded successfully, click **OK** to reset the device.

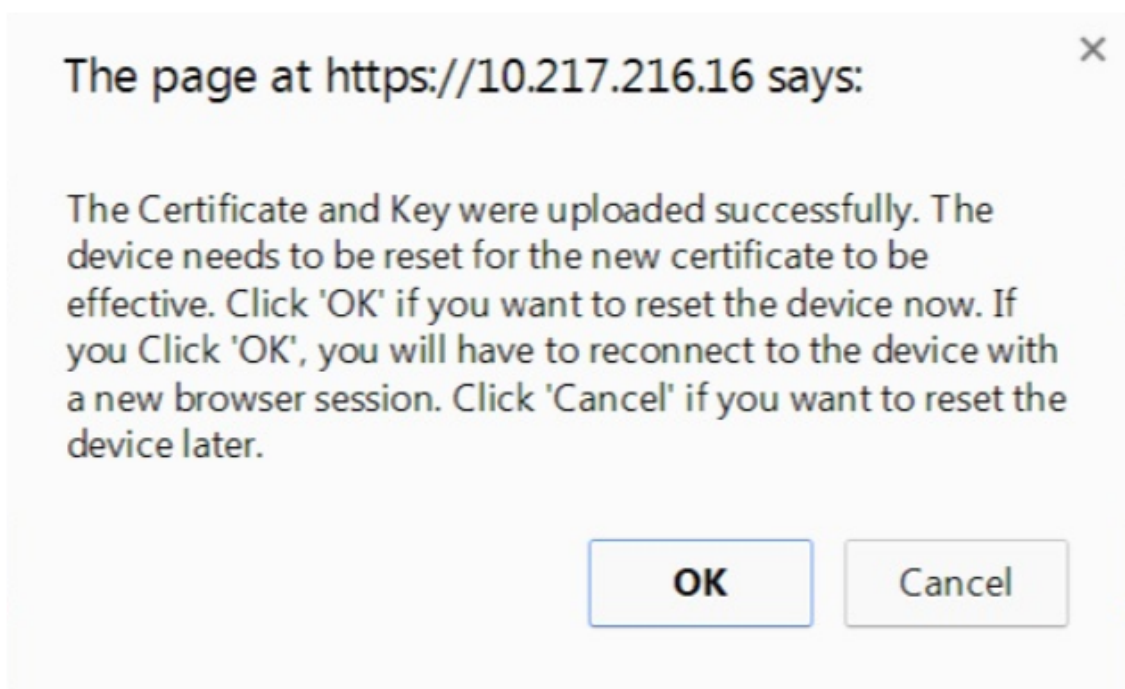

The reset takes approximately 60 seconds. You are then redirected to the logon page.

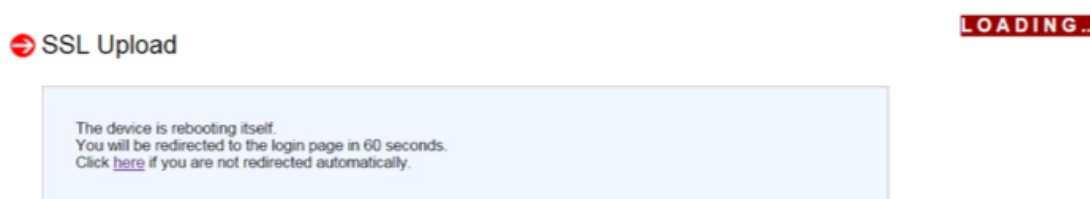


7. Log on to the LOM GUI by using your default credentials.


Note

If the certificate or key is invalid, the BMC reboots, tries the new settings, and reverts to using the previous settings.

8. In the address bar, click the lock icon to display the connection tab, as shown in the following screen.

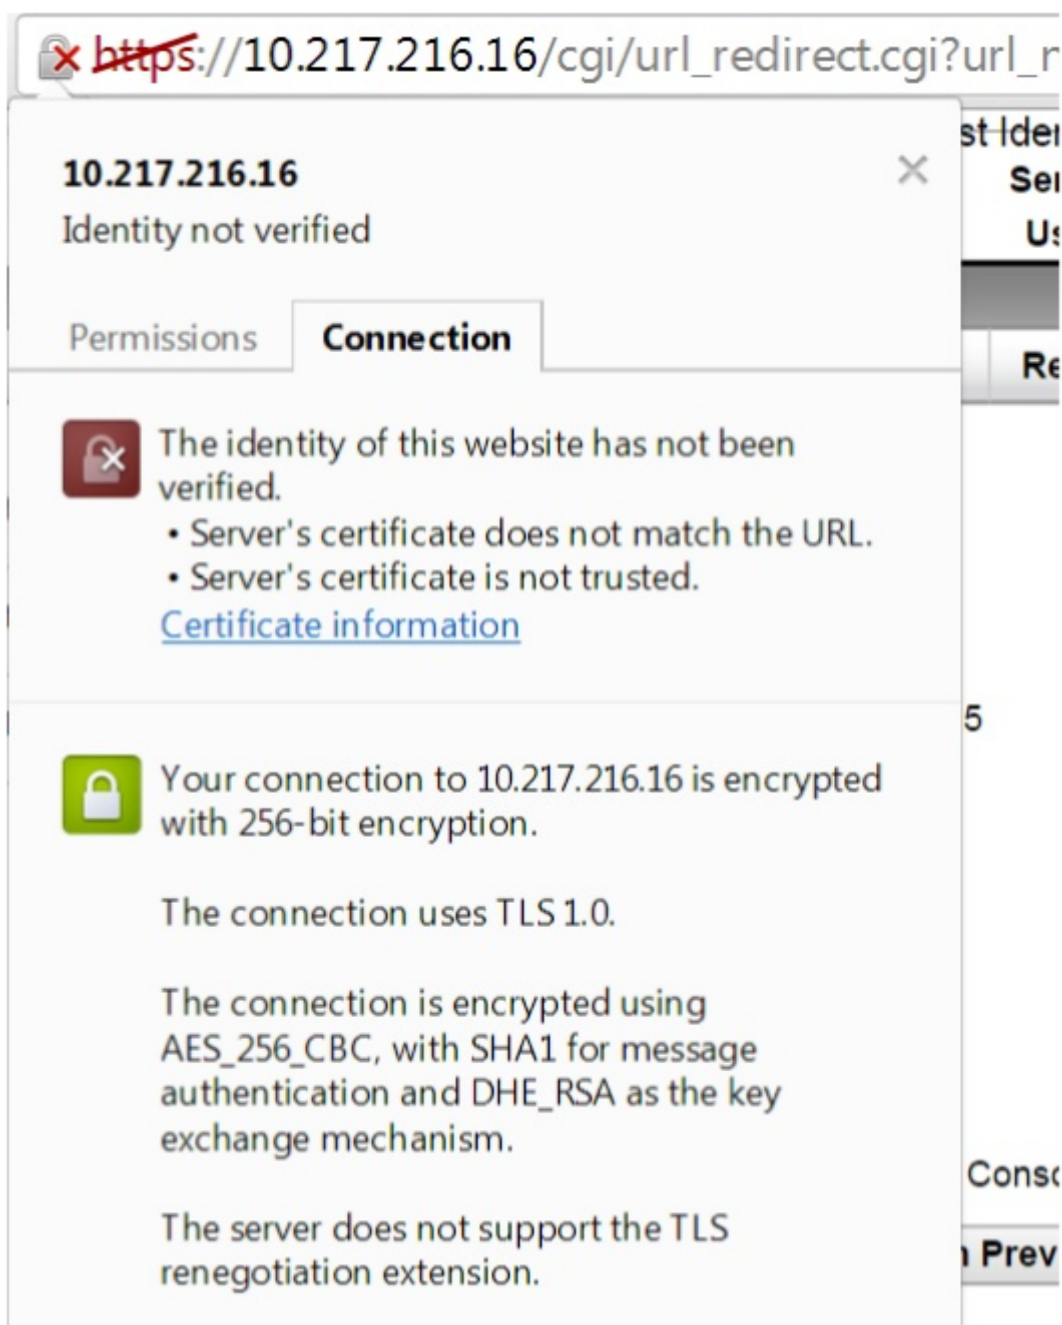

9. Click **Certificate** information to display details about the certificate that you uploaded.

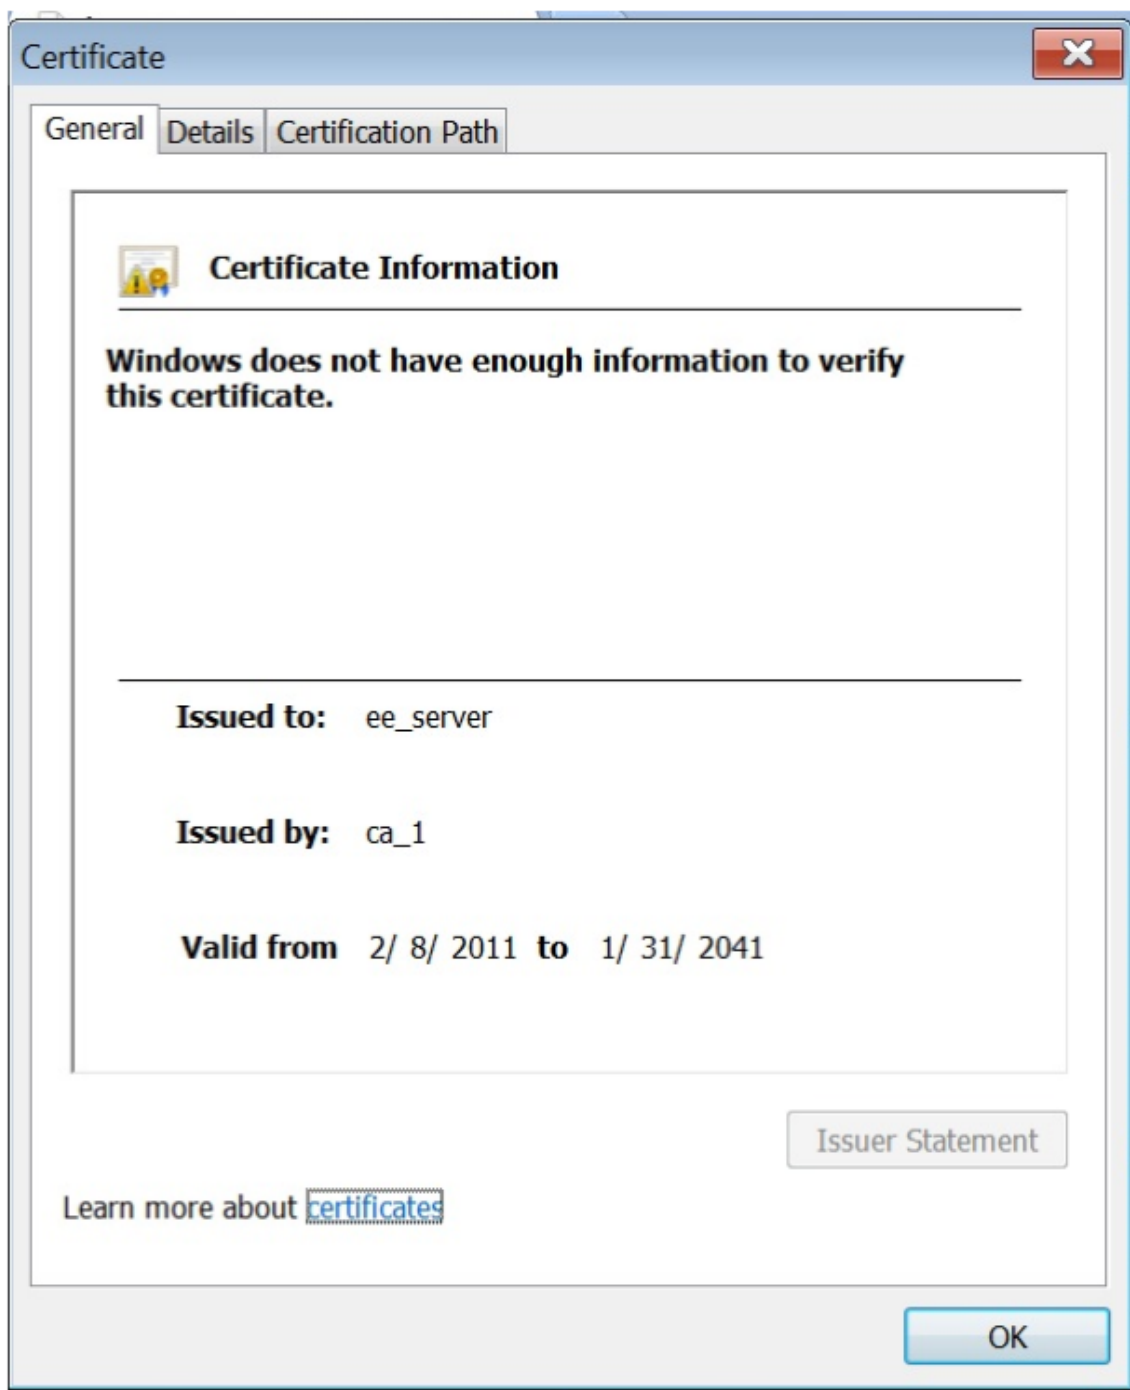

Note: For the best practices for LOM and Citrix ADC security, see <http://support.citrix.com/article/CTX129514>.

Obtaining the MAC address, serial number, and host properties of the appliance

June 24, 2020

A Media Access Control address (MAC address) is a unique identifier assigned to network interfaces for communication on the physical network segment. The serial number is on the back panel of the appliance. If you do not have easy access to the back panel, you can get the appliance's serial number by logging on to the LOM port. You can also retrieve the parameter settings assigned to the IP addresses configured on the appliance, such as the state of ARP, ICMP, telnet, secure shell access, and dynamic routing.

To obtain the MAC address, serial number, and host properties of the appliance by using the LOM GUI

1. In the **Menu** bar, click **Remote Control**.
2. Under **Options**, click **Console Redirection**.
3. Click **Launch Console**, and then click **Yes**.
4. Type the administrator credentials.
5. Type `show interface <management_interface_id>` to display the MAC address.
6. Type `show hardware` to display the serial number of the appliance.
7. Type `sh nsip` to display the host properties of the appliance.

To obtain the MAC address and host properties of the BMC by using the appliance shell

At the shell prompt, type:

```
ipmitool lan print
```

Example

```
1 Set in Progress      : Set Complete
2 Auth Type Support   : MD2 MD5 OEM
3 Auth Type Enable    : Callback : MD2 MD5 OEM
4                     : User      : MD2 MD5 OEM
5                     : Operator  : MD2 MD5 OEM
6                     : Admin    : MD2 MD5 OEM
7                     : OEM      :
8 IP Address Source   : Static Address
9 IP Address          : 192.168.1.3
10 Subnet Mask        : 255.255.255.0
```



```

11 MAC Address           : 00:25:90:3f:5e:d0
12 SNMP Community String : public
13 IP Header             : TTL=0x00 Flags=0x00 Precedence=0x00 TOS=0x00
14 BMC ARP Control      : ARP Responses Enabled, Gratuitous ARP
    Disabled
15 Gratuitous ARP Intrvl : 0.0 seconds
16 Default Gateway IP    : 0.0.0.0
17 Default Gateway MAC   : 00:00:00:00:00:00
18 Backup Gateway IP     : 0.0.0.0
19 Backup Gateway MAC    : 00:00:00:00:00:00
20 802.1q VLAN ID       : Disabled
21 802.1q VLAN Priority  : 0
22 RMCP+ Cipher Suites  : 1,2,3,6,7,8,11,12,0
23 Cipher Suite Priv Max : aaaaXXaaaXXaaXX
24                       : X=Cipher Suite Unused
25                       : c=CALLBACK
26                       : u=USER
27                       : o=OPERATOR
28                       : a=ADMIN
29                       : O=OEM
30
31 <!--NeedCopy-->

```

Perform power control operations by using the LOM port

June 24, 2020

Through the LOM port, you can remotely perform power control operations, such as graceful shut-down and restart, power cycling the appliance, and restarting the BMC microcontroller. A cold restart takes longer than a warm restart. In a cold restart, you switch off power to the appliance and then switch it back on.

Perform power control operations by using the GUI

1. In the **Menu** bar, click **Remote Control**.
2. Under **Options**, click **Power Control**, and then select one of the following options:
 - **Reset System**—Gracefully restart the appliance. All operations on the appliance are stopped, no new connections to the client or server are accepted, and all existing connections are closed before the appliance restarts. This option is similar to a warm restart, such as by entering the reboot command. The BMC does not reboot itself during this operation.

- **Power Off System – Immediate**—Disconnect power to the appliance immediately, without gracefully shutting down the appliance. The BMC continues to operate normally in this mode to allow the user to remotely power on the appliance. This option is the same as pushing the power button until the unit powers off.
- **Power Off System – Orderly Shutdown**—Gracefully shut down the appliance, and then disconnect power to the appliance. Has the same effect as pressing the power button on the back panel of the appliance for less than four seconds. All operations on the appliance are stopped, no new connections to the client or server are accepted, and all existing connections are closed before the appliance shuts down. The BMC continues to operate normally in this mode to allow the user to remotely power on the appliance. This option is the same as entering the shutdown command in the appliance shell.
- **Power On System**—Switch on the appliance. The BMC does not reboot itself during this operation. This option is the same as pushing the power button.
- **Power Cycle System**—Switch off the appliance, and then turn it back on. The BMC does not reboot itself during this operation. This option is the same as pushing the power button until the unit powers off, and then pushing the power button to power on the unit.

3. Click **Perform Action**.

Perform a power cycle of the BMC

A warm restart, cold restart, or a power cycle of the appliance, using the power button, does not include power cycling the BMC. The BMC runs on standby power directly from the power supply. Therefore, the BMC is not affected by any state of the power button on the appliance. The only way to power cycle the BMC is to remove all power cords from the appliance for 60 seconds.

Perform power control operations on the BMC by using the appliance shell

When performing either a warm or cold restart of the BMC microcontroller, you cannot communicate with the LOM port. Both actions restart the BMC but not the main CPU. To perform a warm restart of LOM from the appliance, type:

```
ipmitool mc reset warm
```

Perform a warm restart remotely from another computer on the network

```
ipmitool -U <bmc_gui_username> -P <bmc_gui_password> -H <bmc IP address> mc  
reset warm
```

Perform a cold restart of the LOM from the appliance

```
ipmitool mc reset cold
```

Perform a warm restart remotely from another computer on the network

```
ipmitool -U <bmc_gui_username> -P <bmc_gui_password> -H <bmc IP address> mc  
reset cold
```

Perform a core dump

If the appliance fails or becomes unresponsive, you can remotely perform a core dump. This procedure has the same effect as pressing the **NMI** button on the back panel of the appliance.

Perform a core dump by using the GUI

1. In the **Menu** bar, click **Remote Control**.
2. Under **Options**, click **NMI**, and then click **Initiate NMI**.

Perform a core dump remotely from another computer on the network by using the shell

At the shell prompt, type:

```
ipmitool -U <bmc_gui_username> -P <bmc_gui_password> -H <bmc IP address>  
chassis power diag
```

Restoring the BMC configuration to factory defaults

August 29, 2020

You can restore the BMC to its factory-default settings, including deleting the SSL Certificate and SSL key.

To reset the configuration to factory defaults by using the GUI

1. Navigate to **Maintenance > Factory Default**.
2. Click **Restore**.

To reset the configuration to factory defaults by using the shell

At the shell prompt, type:


```
ipmitool raw 0x30 0x40
```

Specifying the port for IPMI BMC failover

June 24, 2020

With LOM firmware version 3.x or later, the default mode for failover between the dedicated LOM port and the shared LOM/management port is to fail over to the active port. By default, no user configuration is needed other than selecting the port to which to connect the cable. The motherboard has an Ethernet switch between the management MAC and the management port, and between the LOM MAC and the LOM port. The following figure shows the Ethernet switch.

Figure 1. Ethernet Switch

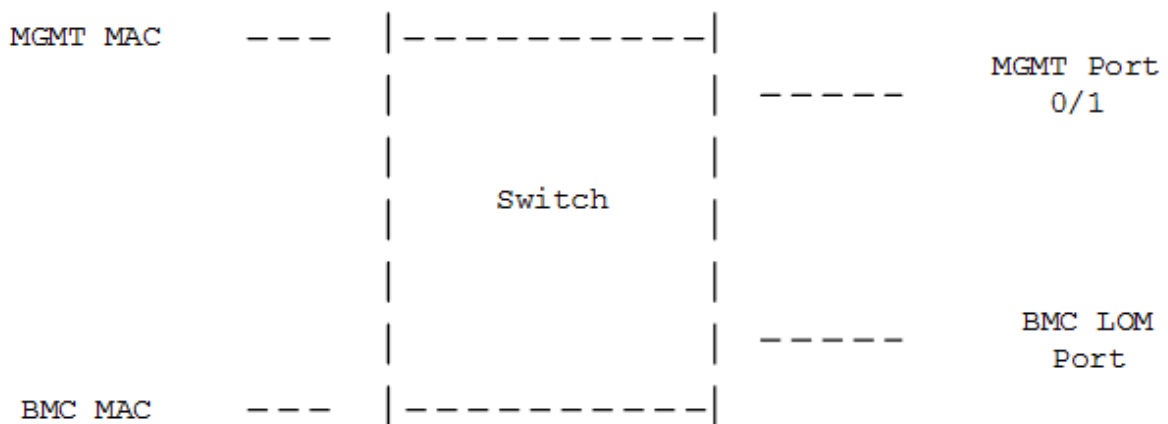

You can set this switch to direct LOM traffic through the dedicated LOM port or through the shared management port. A dedicated LOM port removes the management port as a single point of failure, while a shared LOM/management port reduces the cabling costs.

Using the BIOS POST code to detect errors

February 8, 2021

You can read the BIOS POST code by using the LOM GUI or the shell. To interpret the BIOS Beep codes, see https://www.supermicro.com/manuals/other/AMI_AptioV_BIOS_POST_Codes_for_SM_Motherboards.pdf.

To read the BIOS Post Code by using the LOM GUI

Navigate to **Miscellaneous > BIOS Post Snooping**.

To read the BIOS POST code by using the shell

At the prompt, type:

```
ipmitool raw 0x30 0x2a
```

Hardware health attributes of Citrix ADC SDX appliances

July 15, 2021

Operating ranges for Citrix ADC hardware platforms vary for different attributes.

Note: Use the `stat system -detail` command to display the current values of the attributes.

Health attributes for SDX 80xx/115xx/17500/17550 platforms

The following tables list the health attributes and their recommended value ranges.

Health attributes/- Platform	SNMP Alarm Support	SDX 17500/19500/21550	SDX 115xx	SDX 17550/19550/20550/21550	SDX 8050
CPU 0 core (Volts)	No	0.99–1.5	0.95–1.5	0.95–1.5	- NA -
CPU 1 core (Volts)	No	0.99–1.5	0.95–1.56	0.95–1.5	- NA -
Main 3.3 V Supply (Volts)	Yes	3.19–3.55	3.19–3.55	3.18–3.55	3.14–3.47
Standby 3.3 V Supply (Volts)	Yes	3.2–3.55	3.1–3.55	3.1–3.55	3.14–3.47
+5.0 V Supply (Volts)	No	4.8–5.2	4.8–6.24	4.8–5.2	4.75–5.25
+12.0 V Supply (Volts)	No	11.5–12.35	11.8–12.35	11.5–12.35	11.40–12.60
-12.0 V Supply (Volts)	No	- NA -	- NA -	- NA -	(-10.80)–(-13.20)
Battery (Volts)	No	2.85–3.37	3–3.5	2.8–3.5	> 2.5
Intel CPU Vtt Power (Volts)	No	1–1.2	1–1.2	1–1.2	- NA -

Health attributes/- Platform	SNMP Alarm Support	SDX 17500/19500/21500/SDX 115xx	SDX 17550/19550/20550/SDX 20550	SDX 17550/19550/20550/SDX 20550	SDX 17550/19550/20550/SDX 20550
5 V Standby (Volts)	No	4.88–5.2	4.8–5.25	4.9–5.3	- NA -
Voltage Sensor2 (Volts)	No	1.4–5.2	1.4–6.24	1.4–5.2	3.14–3.47
CPU Fan 0 Speed (RPM)	Yes	3000–16000	3000–16000	3000–16000	> 5500
CPU Fan 1 Speed (RPM)	Yes	3000–16000	3000–16000	3000–16000	> 5500
System Fan Speed (RPM)	Yes	900–15000	900–15000	900–15000	> 5500
System Fan 1 Speed (RPM)	No	900–15000	900–15000	900–16000	> 5500
System Fan 2 Speed (RPM)	No	900–15000	900–15000	900–16000	> 5500
CPU 0 Temperature	Yes	24–90 (Celsius), 75.2–194 (Fahrenheit)	24–90 (Celsius), 75.2–194 (Fahrenheit)	24–90 (Celsius), 75.2–194 (Fahrenheit)	< 85 (Celsius), < 185 (Fahrenheit)
CPU 1 Temperature	Yes	24–90 (Celsius), 75.2–194 (Fahrenheit)	24–90 (Celsius), 75.2–194 (Fahrenheit)	24–90 (Celsius), 75.2–194 (Fahrenheit)	- NA -
Internal Temperature	Yes	19–50 (Celsius), 66.2–122 (Fahrenheit)	19–50 (Celsius), 66.2–122 (Fahrenheit)	19–50 (Celsius), 66.2–122 (Fahrenheit)	< 55 (Celsius), < 131 (Fahrenheit)
Power Supply 1 Status	Yes	Normal	Normal	Normal	Normal
Power Supply 2 Status	Yes	Normal	Normal	Normal	Normal, if both power supplies are installed

Health attributes for the SDX 14000 platform

The following table lists the health attributes for the SDX 14000 platform.

Health Attribute	Recommended Range
CPU 0 core (Volts)	0.85–0.91
CPU 1 core Volt	0.85–0.93
Main 3.3 V Supply (Volts)	3.31–3.36
Standby 3.3 V Supply (Volts)	3.26–3.31
+5.0 V Supply (Volts)	4.99–5.06
+12.0 V Supply (Volts)	11.98–12.08
Battery Voltage	3.02–3.12
Internal CPU Vtt Power	0.99–1.01
CPU Fan 0 Speed (RPM)	1875–4350
CPU Fan 1 Speed (RPM)	1875–4200
System Fan Speed (RPM)	1875–4350
System Fan 1 Speed (RPM)	1875–4275
System Fan 2 Speed (RPM)	1875–4200
CPU 0 Temperature (Celsius)	33–43
CPU 1 Temperature (Celsius)	35–45
Internal Temperature (Celsius)	28–38
Power Supply 1 Status	NORMAL
Power Supply 2 Status	NORMAL

Health attributes for the SDX 22040 platform

The following table lists the health attributes for the SDX 22040 platform.

Health attribute	Unit	Lower		Upper		Upper	
		Non-Recoverable	Critical	Non-Critical	Non-Critical	Critical	Non-Recoverable
CPU1 Temp	degrees C	0.000	0.000	0.000	90.000	93.000	95.000

Health attribute	Unit	Lower		Upper		Upper	
		Non-Recoverable	Lower Critical	Non-Critical	Non-Critical	Upper Critical	Non-Recoverable
CPU2 Temp	degrees C	0.000	0.000	0.000	90.000	93.000	95.000
System Temp	degrees C	-9.000	-7.000	-5.000	80.000	85.000	90.000
Peripheral Temp	degrees C	-9.000	-7.000	-5.000	80.000	85.000	90.000
PCH Temp	degrees C	-11.000	-8.000	-5.000	90.000	95.000	100.000
FPC_Temp 1	degrees C	- NA -	- NA -	- NA -	66.000	70.000	75.000
FPC_Temp 2	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
FPC_Temp 3	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
HDDBP_Temp 1	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
HDDBP_Temp 2	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
FAN 1	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 2	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 3	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 4	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 5	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 6	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 7	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 8	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
PS_1 Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_1 FAN	RPM	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_1 Temp	degrees C	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -

Health attribute	Unit	Lower Non-Recoverable	Lower Critical	Lower Non-Critical	Upper Non-Critical	Upper Critical	Upper Non-Recoverable
PS_2 Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_2 FAN	RPM	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_2 Temp	degrees C	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_3 Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_3 FAN	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
PS_3 Temp	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
PS_4 Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_4 FAN	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
PS_4 Temp	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
FPC Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
VTT	Volts	0.816	0.864	0.912	1.344	1.392	1.440
CPU1 Vcore	Volts	0.480	0.512	0.544	1.488	1.520	1.552
CPU2 Vcore	Volts	0.480	0.512	0.544	1.488	1.520	1.552
VDIMM AB	Volts	1.104	1.152	1.200	1.648	1.696	1.744
VDIMM CD	Volts	1.104	1.152	1.200	1.648	1.696	1.744
VDIMM EF	Volts	1.104	1.152	1.200	1.648	1.696	1.744
VDIMM GH	Volts	1.104	1.152	1.200	1.648	1.696	1.744
+1.5 V	Volts	1.248	1.296	1.344	1.648	1.696	1.744
3.3 V	Volts	2.640	2.784	2.928	3.648	3.792	3.936
+3.3VSB	Volts	2.640	2.784	2.928	3.648	3.792	3.936

Health attribute	Unit	Lower Non-Recoverable	Lower Critical	Lower Non-Critical	Upper Non-Critical	Upper Critical	Upper Non-Recoverable
5 V	Volts	4.096	4.288	4.480	5.504	5.696	6.912
12 V	Volts	10.176	10.494	10.812	13.250	13.568	13.886
VBAT	Volts	2.400	2.544	2.688	3.312	3.456	3.600

Health attributes for SDX 24100 platform

The following table lists the health attributes for SDX 24100/24150.

Health attribute	Unit	Lower Non-Recoverable	Lower Critical	Lower Non-Critical	Upper Non-Critical	Upper Critical	Upper Non-Recoverable
CPU1 Temp	degrees C	0.000	0.000	0.000	90.000	93.000	95.000
CPU2 Temp	degrees C	0.000	0.000	0.000	90.000	93.000	95.000
System Temp	degrees C	-9.000	-7.000	-5.000	80.000	85.000	90.000
Peripheral Temp	degrees C	-9.000	-7.000	-5.000	80.000	85.000	90.000
PCH Temp	degrees C	-11.000	-8.000	-5.000	90.000	95.000	100.000
FPC_Temp 1	degrees C	- NA -	- NA -	- NA -	66.000	70.000	75.000
FPC_Temp 2	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
FPC_Temp 3	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
HDDBP_Temp 1	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
HDDBP_Temp 2	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
FAN 1	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -

Health attribute	Unit	Lower Non-Recoverable	Lower Critical	Lower Non-Critical	Upper Non-Critical	Upper Critical	Upper Non-Recoverable
FAN 2	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 3	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 4	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 5	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 6	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 7	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
FAN 8	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
PS_1 Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_1 FAN	RPM	- NA -	1980.000	- NA -	- NA -	- NA -	- NA -
PS_1 Temp	degrees C	- NA -	- NA -	- NA -	72.000	76.000	82.000
PS_2 Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_2 FAN	RPM	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_2 Temp	degrees C	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_3 Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_3 FAN	RPM	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_3 Temp	degrees C	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_4 Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_4 FAN	RPM	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
PS_4 Temp	degrees C	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
FPC Status	discrete	- NA -	- NA -	- NA -	- NA -	- NA -	- NA -
VTT	Volts	0.816	0.864	0.912	1.344	1.392	1.440

Health attribute	Unit	Lower Non-Recoverable	Lower Critical	Lower Non-Critical	Upper Non-Critical	Upper Critical	Upper Non-Recoverable
CPU1 Vcore	Volts	0.480	0.512	0.544	1.488	1.520	1.552
CPU2 Vcore	Volts	0.480	0.512	0.544	1.488	1.520	1.552
VDIMM AB	Volts	1.104	1.152	1.200	1.648	1.696	1.744
VDIMM CD	Volts	1.104	1.152	1.200	1.648	1.696	1.744
VDIMM EF	Volts	1.104	1.152	1.200	1.648	1.696	1.744
VDIMM GH	Volts	1.104	1.152	1.200	1.648	1.696	1.744
+1.5 V	Volts	1.248	1.296	1.344	1.648	1.696	1.744
3.3 V	Volts	2.640	2.784	2.928	3.648	3.792	3.936
+3.3VSB	Volts	2.640	2.784	2.928	3.648	3.792	3.936
5 V	Volts	4.096	4.288	4.480	5.504	5.696	6.912
12 V	Volts	10.176	10.494	10.812	13.250	13.568	13.886
VBAT	Volts	2.400	2.544	2.688	3.312	3.456	3.600

Health attributes for the SDX 8900 platform

The following table lists the health attributes for the SDX 8900 platform.

Health Attribute	Recommended Range
CPU 0 core (Volts)	1.77–1.81
Main 3.3 V Supply (Volts)	3.25–3.32
Standby 3.3 V Supply (Volts)	3.25–3.32
+5.0 V Supply (Volts)	4.84–4.95
+12.0 V Supply (Volts)	11.75–12.00
Battery (Volts)	3.02–3.13
5 V Standby (Volts)	5.05–5.16
CPU Fan 0 Speed (RPM)	6600–12600

Health Attribute	Recommended Range
CPU Fan 1 Speed (RPM)	6300–12200
System Fan Speed (RPM)	6700–8600
System Fan 1 Speed (RPM)	6600–8500
System Fan 2 Speed (RPM)	6700–8500
CPU 0 Temperature (Celsius)	40–57
CPU 1 Temperature (Celsius)	35–45
Internal Temperature (Celsius)	30–49
Power Supply 1 Status	NORMAL
Power Supply 2 Status	NOT PRESENT–NORMAL

Health attributes for the SDX 15000 and SDX 26000 platforms

The following table lists the health attributes for the SDX 15000 and SDX 26000 platforms.

Health Attribute	Unit	Minimum value	Nominal value	Maximum value
CPU 0 Core Voltage	Volt	1.47	1.82	1.835
CPU 1 Core Voltage	Volt	1.47	1.82	1.835
3_3VCC	Volt	3.12	3.30	3.48
3_3VSB	Volt	3.12	3.30	3.48
5VCC	Volt	4.72	5.00	5.28
p12V	Volt	11.33	12.00	12.67
VBAT	Volt	2.75	3.00	3.200
Vtt	-NA-	-NA-	-NA-	-NA-
5VSB	Volt	4.72	5.00	5.28
Voltage Sensor2	-NA-	-NA-	-NA-	-NA-
CPU Fan 0 Speed	RPM	1500	-NA-	7500
CPU Fan 1 Speed	RPM	1500	-NA-	7500
System Fan Speed	RPM	1500	-NA-	7500

Health Attribute	Unit	Minimum value	Nominal value	Maximum value
System Fan 1 Speed	RPM	1500	-NA-	7500
System Fan 2 Speed	RPM	1500	-NA-	7500
Fan 0 Speed	RPM	1500	-NA-	7500
CPU 0 Temp	Celsius	0	-NA-	85
CPU 1 Temp	Celsius	0	-NA-	85
Internal Temp	Celsius	0	-NA-	80

Fortville NIC firmware upgrade on Citrix ADC SDX appliances

August 29, 2020

Upgrade the firmware on Citrix ADC SDX appliances containing Fortville NICs to remediate <https://support.citrix.com/article/CTX263807>.

Supported platforms

Important: Before upgrading the single bundle image (SBI), first upgrade the VPX instance to one of the following releases:

- Release 11.1 build 65.x and later
- Release 12.1 build 57.x and later
- Release 13.0 build 58.x and later

The firmware and NIC driver are automatically upgraded when the SDX SBI is upgraded to the following minimum versions. The time taken to complete the upgrade varies by platform. For example, on an SDX 14000 platform with 6 Fortville NICs, the total time to upgrade is around 30 min.

Software Version	SBI Version
11.1 build 65.x	11.1 build 65.x
12.1 build 57.x	12.1 build 57.x
13.0 build 58.x	13.0 build 58.x

The following SDX appliances and corresponding zero-capacity appliances contain Fortville NICs:

- SDX 8900
- SDX 14000-40C
- SDX 14000-40S
- SDX 14000-40G
- SDX 15000
- SDX 15000-50G
- SDX 25000-40G
- SDX 26000
- SDX 26000-50S

Converting a Citrix ADC MPX appliance to a Citrix ADC SDX appliance

August 29, 2020

You can convert a Citrix ADC MPX appliance to an SDX appliance to deploy multiple virtualized ADC instances on a single, purpose-built physical appliance with full multiservice and multitenant support.

Note: Conversion of an SDX appliance to an MPX appliance is not supported.

You can convert the Citrix ADC MPX 11515/11520/11530/11540/11542 appliances to Citrix ADC SDX 11515/11520/11530/11540/11542 appliances. To convert, upgrade the software through a new Solid State Drive (SSD) and a new Hard Disk Drive (HDD).

The Citrix ADC models SDX 11515/11520/11530/11540/11542 are 2U appliances. Each model has two 6-core processors for a total of 12 physical cores (24 cores with hyper-threading), and 48 GB of memory.

The SDX 11515/11520/11530/11540/11542 appliances have the following ports:

- RS232 serial console port.
- 10/100Base-T copper Ethernet Port (RJ45), also called the LOM port. You can use this port to remotely monitor and manage the appliance independently of the Citrix ADC software.

Note:

On the SDX 11515/11520/11530/11540/11542 appliances, the LEDs on the LOM port are not operational, by design.

- Two 10/100/1000Base-T copper Ethernet management ports (RJ45), numbered 0/1 and 0/2 from left to right. These ports are used to connect directly to the appliance for system administration functions. Eight 10G SFP+ ports and four copper or fiber 1G SFP ports.

You can convert the Citrix ADC MPX 8005/8010/8015/8200/8400/8600/8800 appliances to Citrix ADC SDX 8010/8015/8400/8600 appliances by upgrading the software through a new Solid State Drive (SSD).

The Citrix ADC models SDX 8010/8015/8400/8600 are 1U appliances. Each model has one quad-core processor (8 cores with hyper-threading) and 32 GB of memory. The SDX 8010/8015/8400/8600 appliances are available in two port configurations:

- Six 10/100/1000Base-T copper Ethernet ports and six 1G SFP ports (6x10/100/1000Base-T copper Ethernet ports + 6x1G SFP)
- Six 10/100/1000Base-T copper Ethernet ports and two 10G SFP+ ports (6x10/100/1000Base-T copper Ethernet ports + 2x10G SFP+)

Converting a Citrix ADC MPX 11515/11520/11530/11540/11542 appliance to a Citrix ADC SDX 11515/11520/11530/11540/11542 appliance

August 11, 2020

You can convert a Citrix ADC MPX appliance to a Citrix ADC SDX appliance by upgrading the software through a new Solid State Drive (SSD) and a new Hard Disk Drive (HDD). Citrix supplies a field conversion kit to migrate a Citrix ADC MPX appliance to a Citrix ADC SDX appliance.

Note

Citrix recommends that you configure the lights out management (LOM) Port of the Citrix ADC appliance before starting the conversion process. For more information on the LOM port of the Citrix ADC appliance, see [Lights out management port of the Citrix ADC appliance](#).

To convert a Citrix ADC MPX appliance to a Citrix ADC SDX appliance, you must access the appliance through a console cable attached to a computer or terminal. Before connecting the console cable, configure the computer or terminal to support the following configuration:

- VT100 terminal emulation
- 9600 baud
- 8 data bits
- 1 stop bit
- Parity and flow control set to NONE

Connect one end of the console cable to the RS232 serial port on the appliance, and the other end to the computer or terminal.

Note


To use a cable with an RJ-45 converter, insert the optional converter into the console port and attach the cable to it.

With the cable attached, verify that the MPX appliance's components are functioning correctly. You are then ready to begin the conversion. The conversion process modifies the BIOS, installs Citrix Hypervisor and a Service Virtual Machine image, and copies the Citrix ADC VPX image to the Hard Disk Drive.

After the conversion process, you make a few modifications to the appliance's configuration and apply a new license. You can then provision the VPX instances through the Management Service on what is now a Citrix ADC SDX appliance.

The following figure shows the front panel of the MPX 11515/11520/11530/11540/11542 appliance.

Figure 1. Citrix ADC MPX 11515/11520/11530/11540/11542, front panel

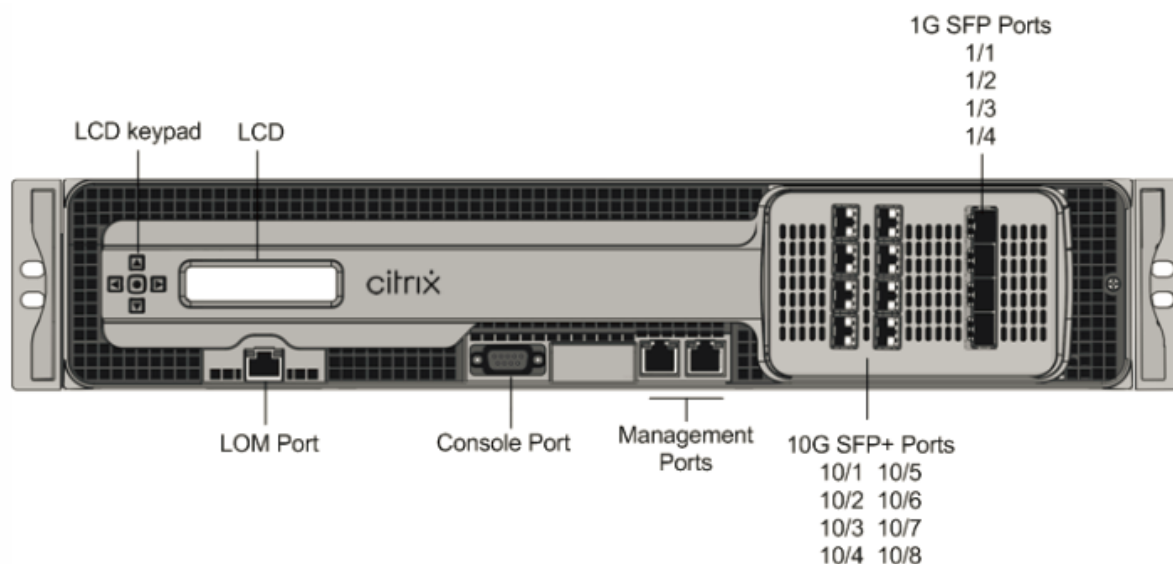**To verify proper operation of the MPX appliance's components**

1. Access the console port and enter the administrator credentials.
2. Run the following command from the command line interface of the appliance to display the serial number: `show hardware`

The serial number might be helpful in case you want to contact Citrix Technical Support.

Example

```

1 > show hardware
2 Platform: NSMPX-11500 12*CPU+8*IX+4*E1K+2*E1K+2*CVM N3
1400210

```

```

3      Manufactured on: 8/12/2014
4      CPU: 2400MHZ
5      Host Id: 872841350
6      Serial no: 2NSHJ2DR9E
7      Encoded serial no: 2NSHJ2DR9E
8 Done
9 <!--NeedCopy-->

```

- Run the following command to display the status of the active 1G and 10G interfaces: `show interface`
- In the show interface command's output, verify that all of the interfaces are enabled and the status of every interface is shown as UP/UP.

Note: If you do not have an SFP+ transceiver for every port, verify the interfaces in stages. After checking the first set of interfaces, unplug the SFP+ transceivers and plug them in to the next set of ports. The SFP+ transceivers are not hot-swappable. Therefore, restart the MPX appliance after you connect the transceivers.

- Run the following commands for each of the interfaces that are not in the UP/UP state where x is the new interface number.

```

1      - enable interface 1/x
2      - enable interface 10/x
3 <!--NeedCopy-->

```

- Run the following command to verify that the status of the power supplies is normal: `stat system -detail`

Example:

```

1 > stat system -detail
2 NetScaler Executive View
3 System Information:
4 Up since      Wed Aug 13 12:09:54 2014
5 Memory usage (MB)          924
6 InUse Memory (%)          5.64
7 Number of CPUs            5
8
9 System Health Statistics (Standard):
10 CPU 0 Core Voltage (Volts)      1.10
11 CPU 1 Core Voltage (Volts)      1.10
12 Main 3.3 V Supply Voltage      3.26
13 Standby 3.3 V Supply Voltage    3.22
14 +5.0 V Supply Voltage           5.09
15 +12.0 V Supply Voltage          12.14

```

```
16 Battery Voltage (Volts) 3.17
17 Intel CPU Vtt Power(Volts) 0.00
18 5V Standby Voltage(Volts) 4.97
19 Voltage Sensor2(Volts) 0.00
20 CPU Fan 0 Speed (RPM) 5929
21 CPU Fan 1 Speed (RPM) 5929
22 System Fan Speed (RPM) 5929
23 System Fan 1 Speed (RPM) 5929
24 System Fan 2 Speed (RPM) 5929
25 CPU 0 Temperature (Celsius) 49
26 CPU 1 Temperature (Celsius) 51
27 Internal Temperature (Celsius) 33
28 Power supply 1 status NORMAL
29 Power supply 2 status NORMAL
30
31 System Disk Statistics:
32 /flash Size (MB) 63473
33 /flash Used (MB) 149
34 /flash Available (MB) 58246
35 /flash Used (%) 0
36 /var Size (MB) 745163
37 /var Used (MB) 249
38 /var Available (MB) 685300
39 /var Used (%) 0
40
41 System Health Statistics(Auxiliary):
42 Voltage 0 (Volts) 0.00
43 Voltage 1 (Volts) 0.00
44 Voltage 2 (Volts) 0.00
45 Voltage 3 (Volts) 0.00
46 Voltage 4 (Volts) 1.50
47 Voltage 5 (Volts) 0.00
48 Voltage 6 (Volts) 0.00
49 Voltage 7 (Volts) 0.00
50 Fan 0 Speed (RPM) 5929
51 Fan 1 Speed (RPM) 0
52 Fan 2 Speed (RPM) 0
53 Fan 3 Speed (RPM) 0
54 Temperature 0 (Celsius) 40
55 Temperature 1 (Celsius) 35
56 Temperature 2 (Celsius) 0
57 Temperature 3 (Celsius) 0
58 Done
59 <!--NeedCopy-->
```

2. Run the following command to generate a tar of system configuration data and statistics: `show techsupport`

Example:

```
1 > show techsupport
2 showtechsupport data collector tool - $Revision: #1 $! NetScaler
   version 9.2
3 The NS IP of this box is 10.10.10.10
4 Current HA state: Primary (or this is not part of HA
5 pair!)
6 All the data will be collected under
7
8 /var/tmp/support/collector_10.10.10.10_P_13May2011_12_01
9 Copying selected configuration files from nsconfig ....
10 <!--NeedCopy-->
```

Note: The output of the command is available in the `/var/tmp/support/collector_<IP_address>_P_<date>.tar.gz` file. Copy this file to another computer for future reference. The output of the command might be helpful in case you want to contact Citrix Technical Support.

3. At the Citrix ADC command line interface, switch to the shell prompt. Type: `shell`
4. Run the following command to verify that 2 Cavium cards are available: `root@ns## dmesg | grep cavium`

Example:

```
1 root@ns# dmesg | grep cavium
2 Cavium cavium_probe : found card 0x177d,device=0x11
3 cavium0 mem 0xdd000000-0xddffffff irq 24 at device 0.0 on pci20
4 Cavium cavium_probe : found card 0x177d,device=0x11
5 cavium1 mem 0xd6f00000-0xd6ffffff irq 32 at device 0.0 on pci5
6 <!--NeedCopy-->
```

Run the following command to verify that 596 MB of RAM is reserved for shared memory:

```
root@ns## dmesg | grep memory
```

Example:

```
1 root@ns# dmesg | grep memory
2 real memory = 52613349376 (50176 MB)
3 avail memory = 49645355008 (47345 MB)
4 NS-KERN map_shared_mem_ioctl (cpu 7, NSPPE-03): Reserving 596 MB
   for shared memory type 0
5 <!--NeedCopy-->
```

5. Run the following command to verify that the appliance has 12 CPU cores: `root@ns## dmesg | grep cpu`

Example:

```
1 root@ns# dmesg | grep cpu
2 cpu0 (BSP): APIC ID: 0
3 cpu1 (AP): APIC ID: 2
4 cpu2 (AP): APIC ID: 4
5 cpu3 (AP): APIC ID: 16
6 cpu4 (AP): APIC ID: 18
7 cpu5 (AP): APIC ID: 20
8 cpu6 (AP): APIC ID: 32
9 cpu7 (AP): APIC ID: 34
10 cpu8 (AP): APIC ID: 36
11 cpu9 (AP): APIC ID: 48
12 cpu10 (AP): APIC ID: 50
13 cpu11 (AP): APIC ID: 52
14 cpu0: <ACPI CPU> on acpi0
15 acpi_throttle0: <ACPI CPU Throttling> on cpu0
16 cpu1: <ACPI CPU> on acpi0
17 acpi_throttle1: <ACPI CPU Throttling> on cpu1
18 cpu2: <ACPI CPU> on acpi0
19 cpu3: <ACPI CPU> on acpi0
20 cpu4: <ACPI CPU> on acpi0
21 cpu5: <ACPI CPU> on acpi0
22 cpu6: <ACPI CPU> on acpi0
23 cpu7: <ACPI CPU> on acpi0
24 cpu8: <ACPI CPU> on acpi0
25 cpu9: <ACPI CPU> on acpi0
26 cpu10: <ACPI CPU> on acpi0
27 cpu11: <ACPI CPU> on acpi0
28 NS-KERN map_shared_mem_ioctl (cpu 7, NSPPE-03): Reserving 596 MB
    for shared memory type 0
29 <!--NeedCopy-->
```

6. Run the following command to verify that the /var drive is mounted as /dev/ad8s1e: `root@ns ## df -h`

Example:

```
1 root@ns# df -h
2 Filesystem      Size    Used    Avail Capacity  Mounted on
3 /dev/md0c       276M   246M     24M     91%      /
4 devfs           1.0K    1.0K     0B    100%     /dev
5 procfs          4.0K    4.0K     0B    100%     /proc
```

```
6 /dev/ad4s1a      62G    149M    57G    0%    /flash
7 /dev/ad8s1e     728G   299M    669G   0%    /var
8 root@ns#
9
10 <!--NeedCopy-->
```

7. Type the following command to run the ns_hw_err.bash script, which checks for latent hardware errors: root@ns## /netscaler/ns_hw_err.bash

Example:

```
1 root@ns# /netscaler/ns_hw_err.bash
2 NetScaler NS10.1: Build 127.11.nc, Date: Aug 11 2014, 18:24:36
3 platform: serial 2NSHJ2DR9E
4 platform: sysid 1400210 - NSMPX-11500 12*CPU+8*IX+4*E1K+2*E1K+2*
   CVM N3
5 HDD MODEL: Device Model:      ST1000NM0033-9ZM173
6
7 Generating the list of newslog files to be processed...
8 Generating the events from newslog files...
9 Checking for HDD errors...
10 /var/nslog/dmesg.prev:swap.NO
11 *****
12 HDD ERROR: FOUND           1 HDD errors: swap.NO
13 *****
14 Checking for HDD SMART errors...
15 Checking for Flash errors...
16 Checking for SSL errors...
17 Checking for BIOS errors...
18 Checking for SMB errors...
19 Checking for MotherBoard errors...
20 Checking for CMOS errors...
21      License year: 2014: OK
22 License server failed at startup. Check /var/log/license.log
23 Vendor daemon failed at startup. Check /var/log/license.log
24 Checking for SFP/NIC errors...
25 Checking for Firmware errors...
26 Checking for License errors...
27 Checking for Undetected CPUs...
28 Checking for DIMM flaps...
29 Checking the Power Supply Errors...
30 root@ns#
31
32 <!--NeedCopy-->
```


8. **Important:** Physically disconnect all ports except the LOM port, including the management port, from the network.
9. At the shell prompt, switch to the Citrix ADC command line. Type: `exit`
10. Run the following command to shut down the appliance: `shutdown -p now`

Example:

```
1 > shutdown -p now
2 Are you sure you want to completely stop NetScaler (Y/N)? [N]:y
3 <!--NeedCopy-->
```

To upgrade the appliance

1. Locate the solid-state drive on the back panel of the appliance, as shown in the following figure:

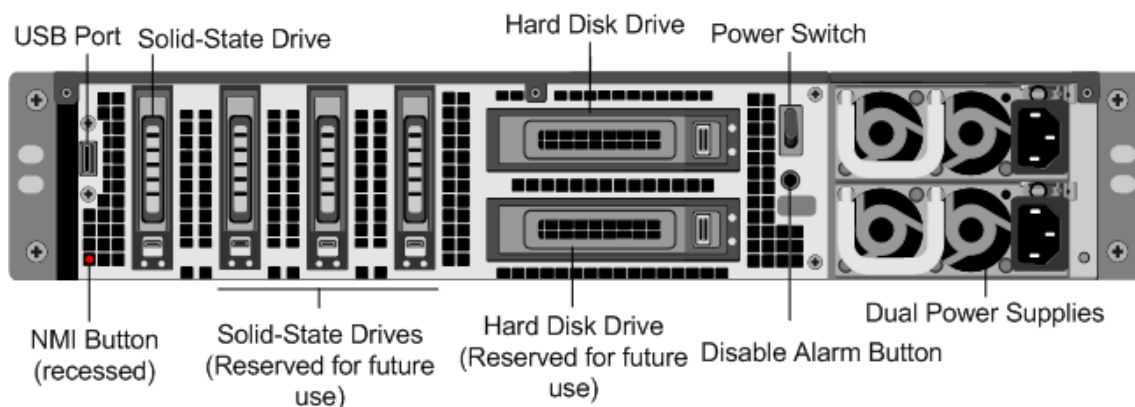

2. Verify that the replacement solid-state drive (SSD) is the one required for your Citrix ADC model. The Citrix label is on the top of the solid-state drive, which is pre-populated with a new version of BIOS and a recent build of the required Service VM software.
3. Remove the SSD drive by pushing the safety latch of the drive cover down while pulling the drive handle.
4. On the new SSD drive, open the drive handle completely, and then insert the new drive into the slot.
5. Close the handle flush with the rear side of the appliance so that the drive locks securely into the slot.
Important: The orientation of the solid-state drive is important. When you insert the drive, make sure that the Citrix product label is at the top.
6. Locate the hard disk drive (HDD) on the back panel of the appliance.
7. Remove the HDD by pushing the safety latch of the drive cover to the right and pulling the drive handle.

8. On the new disk drive, open the drive handle completely to the left, and then insert the new drive into the slot.
9. Close the handle flush with the rear side of the appliance so that the hard drive locks securely into the slot.
10. Store the old SSD/HDD pair for future handling.

Important: The orientation of the hard disk drive is important. When you insert the drive, make sure that the Citrix product label is at the top.

11. Start the Citrix ADC appliance. For instructions, see the Switching on the Appliance section in [Installing the hardware](#) ([/en-us/citrix-hardware-platforms/sdx/installing-the-hardware.html](#)).

The conversion process takes approximately 30 minutes to complete. The conversion process updates the BIOS, installs the Citrix Hypervisor and the Management Service Operating system, and copies the Citrix ADC VPX image to the hard disk drive for instance provisioning. When the conversion begins, the LCD screen on the front bezel indicates NSMPX-11500 10G, as shown in the following figure.



When the conversion is successful, the LCD indicates Citrix NSSDX - 11515, as shown in the following figure.



Note: The serial number of the appliance remains the same.

12. Keep the console cable attached during the conversion process. Allow the process to complete, at which point the `netcaler-sdx login:` prompt appears.

If the boot SSD is not inserted completely into the designated slot, the Citrix ADC SDX appliance attempts to start from the hard disk drive, and the bootup process results in a prompt different from the one mentioned earlier. If the `netcaler-sdx login:` prompt does not appear, carefully reseal the SSD, close the locking handle, and restart the appliance.

Converting a Citrix ADC MPX 8005/8010/8015/8200/8400/8600/8800 appliance to a Citrix ADC SDX 8010/8015/8400/8600 appliance

August 11, 2020

To convert a Citrix ADC MPX 8005 appliance to a Citrix ADC SDX 8010 appliance, access the appliance through a console cable attached to a computer or terminal.

Before connecting the console cable, configure the computer or terminal to support the following configuration:


1. VT100 terminal emulation
2. 9600 baud
3. 8 data bits
4. 1 stop bit
5. Parity and flow control set to NONE

To convert a Citrix ADC MPX 8005/8010/8015/8200/8400/8600/8800 appliance to a Citrix ADC SDX 8010/8015/8400/8600 appliance

1. Connect one end of the console cable to the RS232 serial port on the appliance and the other end to the computer or terminal.

Note:

To use a cable with an RJ45 converter, insert the optional converter into the console port and attach the cable to it.

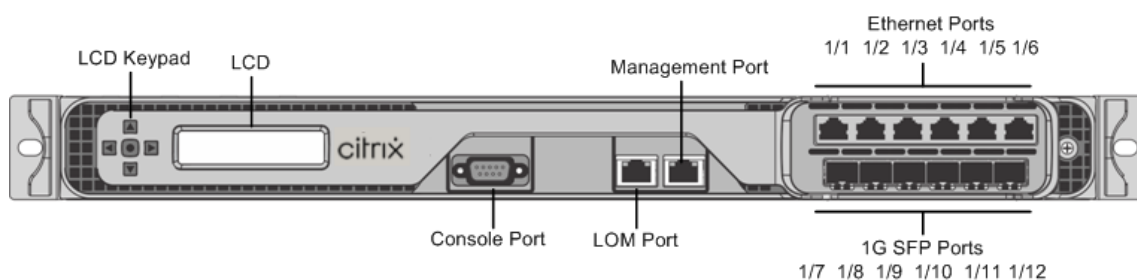

2. On the Citrix ADC MPX appliance, verify that the solid state drive, power supplies, CPU, SSL cores, and interfaces are operational.
3. Access the console port and enter the administrator credentials.
4. Run the following command from the Citrix ADC command line interface to display the serial number and confirm the SYSID of the appliance: `show hardware`
5. Run the following command to display the status of the active interfaces: `show interface`

6. In the `show interface` command's output, verify that all the interfaces are enabled and the status of every interface is shown as UP/UP.

Note:

If you have only a limited number of SFP+ transceivers, verify the interfaces in stages. After checking the first set of interfaces, unplug the SFP+ transceivers and plug them in to the next set of ports. The SFP+ transceivers are not hot-swappable. Therefore, restart the MPX appliance after you connect the transceivers.

7. Run the following commands for each of the interfaces:

```
enable interface 1/x
```

```
enable interface 10/x
```

where x is the new interface number.

8. For any interface that you do not want to use after conversion, run the following commands:

```
disable interface 1/x
```

```
disable interface 10/x
```

9. Run the following command to verify that the status of the power supplies is normal: `stat system -detail`


10. Run the following command: `show techsupport`

Note:


The output of the command is available in the `/var/tmp/support/collector_<IP_address>_P_<date>.tar.gz` file. Copy this file to another computer for future reference. It might be helpful if you want to contact a Citrix technical support engineer.

11. At the Citrix ADC command line interface, switch to the shell prompt. Type: `shell`
12. Run the following command to verify that 4 Cavium cores are available: `root@ns## dmesg | grep cavium`
13. Run the following command to verify that 132 MB of RAM is reserved for shared memory: `root@ns## dmesg | grep memory`
14. Run the following command to verify that the appliance has 4 CPU cores: `root@ns## dmesg | grep cpu`
15. Run the following command to verify that the /var drive is mounted as /dev/ad4s1e: `root@ns## df -h`
16. Enter the following command to run the `ns_hw_err.bash` script. This script checks for latent hardware errors. `root@ns## /netscaler/ns_hw_err.bash`

17. At the shell prompt, switch to the Citrix ADC command line interface. Type: `exit`
18. Run the following command to shut down the appliance: `shutdown -p now`
19. Locate the solid-state drive on the back panel of the appliance, as shown in the following figure:

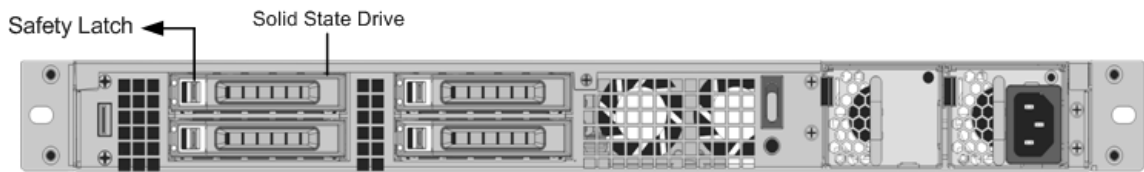

20. Verify that the replacement solid-state drive is the one required for your Citrix ADC model. The Citrix label is on the top of the solid-state drive. The SSD is pre-populated with a new version of the BIOS, and a recent build of the required Service VM software.
21. Remove the currently installed SSD drive by pushing the safety latch of the drive cover to the right and removing the drive handle and the existing drive.
22. Open the drive handle on the new drive completely to the left, and insert the drive into the slot. The following figure shows the drive partially inserted. Push the drive all the way into the slot.

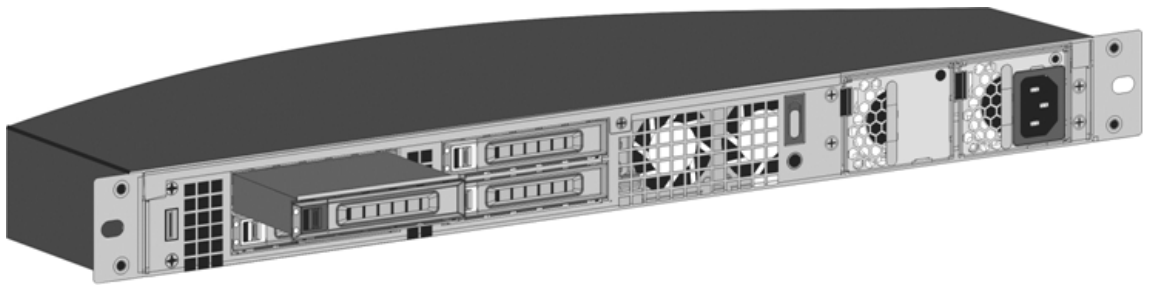

23. Close the handle flush with the rear side of the appliance so that the solid-state drive locks securely into the slot.

Important:

The orientation of the solid-state drive is important. Make sure that the Citrix product label is facing up when you insert the drive.

24. Store the old SSD.
25. Start the Citrix ADC appliance. It takes approximately 30 minutes for the conversion process to complete. The conversion process performs the following actions:
 - Updates the BIOS.
 - Installs the Citrix Hypervisor and the Service VM operating system.
 - Copies the Citrix ADC VPX image to the solid state drive for instance provisioning.

When the conversion begins, the LCD screen on the front panel indicates NSMPX-8200 Booting... or NSMPX-8200 10G Booting... depending on the model of the appliance. When the conversion is suc-

successful, the LCD indicates Citrix NSSDX-8200 or Citrix NSSDX-8200 10G, depending on the model of the appliance.

```
1 > **Note:**
2 >
3 > The serial number of the appliance remains the same.
```

1. Keep the console cable attached during the conversion process. Allow the process to continue until the netcaler-sdx login: prompt appears.
2. When the appliance finishes the conversion process, it no longer has the previously working configuration. Therefore, you can access the appliance through a Web browser only. Use the default IP address: 192.168.100.1/16. Configure a computer on network 192.168.0.0 and connect it directly to the management port 0/1 of the appliance by using a cross-over Ethernet cable. Alternatively, access the Citrix ADC SDX appliance through a network hub by using a straight-through Ethernet cable. Use the default credentials.
3. Select the **Configuration** tab.
4. Verify that the **System Resource** section displays 8 CPU cores, 4 SSL cores, and 32 GB of total memory for the Citrix ADC SDX appliance.
5. Select **System node** and click the Network Configuration link on the System page to modify the IP address of the Service VM.
6. In the **Modify Network Configuration** dialog box, specify the following details:
 - Interface—The interface through which clients connect to the Management Service. Possible values: 0/1, 0/2. Default: 0/1.
 - Citrix Hypervisor IP Address—The IP address of Citrix Hypervisor.
 - Management Service IP Address—The IP address of the Management Service.
 - Netmask—The subnet mask for the subnet in which the SDX appliance is located.
 - Gateway—The default gateway for the network.
 - DNS Server—The IP address of the DNS server.

*An optional parameter
7. Click **OK**.
8. Connect the Citrix ADC SDX appliance to a switch to access it through the network. Browse to the Management Service IP address defined in step 31 and log on with the default credentials.
9. For instructions for applying the licenses, see [Citrix ADC SDX Licensing Overview](#).

Converting a Citrix ADC MPX 24100 and 24150 appliance to a Citrix ADC SDX 24100 and 24150 appliance

August 18, 2020

You can convert a Citrix ADC MPX appliance to a Citrix ADC SDX appliance by upgrading the software through a new Solid State Drive (SSD). Citrix supplies a field conversion kit to migrate a Citrix ADC MPX appliance to a Citrix ADC SDX appliance.

The conversion requires minimum of four SSDs.

Note

Citrix recommends that you configure the lights out management (LOM) Port of the Citrix ADC appliance before starting the conversion process. For more information on the LOM port of the Citrix ADC appliance, see [Lights out Management Port of the Citrix ADC appliance](#).

To convert a Citrix ADC MPX appliance to a Citrix ADC SDX appliance, you must access the appliance through a console cable attached to a computer or terminal. Before connecting the console cable, configure the computer or terminal to support the following configuration:

- VT100 terminal emulation
- 9600 baud
- 8 data bits
- 1 stop bit
- Parity and flow control set to NONE

Connect one end of the console cable to the RS232 serial port on the appliance, and the other end to the computer or terminal.

Note

To use a cable with an RJ-45 converter, insert the optional converter into the console port and attach the cable to it.

Citrix recommends you to connect a VGA monitor to the appliance to monitor the conversion process, because the LOM connection is lost during the conversion process.

With the cable attached, verify that the MPX appliance's components are functioning correctly. You are then ready to begin the conversion. The conversion process modifies the BIOS, installs Citrix Hypervisor and a Management Service image, and copies the Citrix ADC VPX image to the Solid State Drive.

The conversion process also sets up a Redundant Array of Independent Disks (RAID) controller for local storage (SSD slot # 1 and SSD slot # 2) and Citrix ADC VPX storage (SSD slot # 3 and SSD slot # 4).

After the conversion process, modify the appliance's configuration and apply a new license. You can then provision the VPX instances through the Management Service on what is now a Citrix ADC SDX appliance.

To verify proper operation of the MPX appliance's components

1. Access the console port and enter the administrator credentials.
2. Run the following command from the command line interface of the appliance to display the serial number:
`show hardware`
The serial number might be helpful if you want to contact Citrix Technical Support.
3. Run the following command to display the status of the active 10G interfaces: `show interface`
4. In the `show interface` command's output, verify that all the interfaces are enabled and the status of every interface is shown as UP/UP.


Note

If you do not have an SFP+ transceiver for every port, verify the interfaces in stages. After checking the first set of interfaces, unplug the SFP+ transceivers and plug them in to the next set of ports.

5. Run the following command for each of the interfaces that are not in the UP/UP state:

To upgrade the appliance

1. Power off the Citrix ADC appliance.
2. Locate two solid-state drives (SSDs) on the back of the appliance in slot #1 and slot #2, as shown in the following figure:

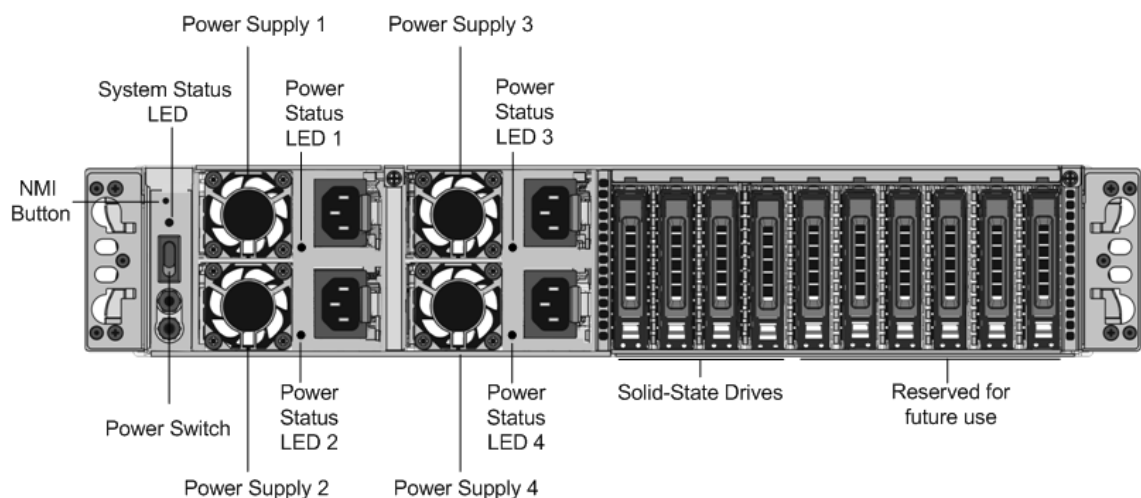

3. Verify that the replacement solid-state drives (SSDs) are the ones required for your Citrix ADC model. The conversion requires minimum of four SSDs. The Citrix label is on the top of one of the solid-state drives, which is pre-populated with a new version of BIOS and a recent build of the required Citrix ADC SDX Management Service. This SSD must be installed in slot # 1.
4. Remove the SSDs by pushing the safety latch of the drive cover down while pulling the drive handle.
5. On the new Citrix Certified SSD drive, open the drive handle completely to the left, and then insert the new drive into the slot #1 as far as possible.
6. To seat the drive, close the handle flush with the rear side of the appliance so that the drive locks securely into the slot.

Important

The orientation of the SSD is important. When you insert the drive, make sure that the Citrix product label is at the top.

7. Insert a second Citrix certified SSD, which matches the capacity of the SSD in slot #1, in slot # 2. Insert more blank Citrix certified SSDs in slots #3 and #4.

Important

Mixing and matching of old and new SSDs is not supported. SSDs in slot #1 and slot # 2, which constitute the first RAID pair (local storage), must be of the same size and type. Similarly, SSDs in slot # 3 and slot #4, which constitute the second RAID pair (VPX storage), must be of the same size and type. Only use drives that are part of the provided conversion kit.

8. Disconnect all network cables from the data ports and the management ports.
9. Start the Citrix ADC appliance. For instructions, see “Switching on the Appliance” in Installing the Hardware. The conversion process can run for approximately 30 minutes, during which you must not power cycle the appliance. The entire conversion process might not be visible on the console and might appear to be unresponsive. The conversion process updates the BIOS, installs the Citrix Hypervisor and the Management Service. It also copies the Citrix ADC VPX image to the SSD for instance provisioning, and forms the Raid1 pair.

Note

The serial number of the appliance remains the same.

10. Keep the console cable attached during the conversion process. Allow the process to complete, at which point the netscaler-sdx login: prompt appears.
11. During the conversion process the LOM port connection might be lost as it resets the IP address to the default value of 192.168.1.3. The conversion status output is available on the VGA monitor.

Convert a Citrix ADC MPX 14020/14030/14040/ 14060/14080/14100 appliance to a Citrix ADC SDX 14020/14030/14040/ 14060/14080/14100 appliance

August 11, 2020

You can convert a Citrix ADC MPX appliance to a Citrix ADC SDX appliance by upgrading the software through a new solid-state drive (SSD). Citrix supplies a field conversion kit to migrate a Citrix ADC MPX appliance to an SDX appliance.

The conversion requires minimum of four SSDs.

Note: Citrix recommends that you configure the lights out management (LOM) port of the Citrix ADC appliance before starting the conversion process. For more information on the LOM port of the Citrix ADC appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

To convert a Citrix ADC MPX appliance to an SDX appliance, you must access the appliance through a console cable attached to a computer or terminal. Before connecting the console cable, configure the computer or terminal to support the following configuration:

- VT100 terminal emulation
- 9600 baud
- 8 data bits
- 1 stop bit
- Parity and flow control set to NONE

Connect one end of the console cable to the RS232 serial port on the appliance, and the other end to the computer or terminal.

Note: To use a cable with an RJ-45 converter, insert the optional converter into the console port and attach the cable to it.

Citrix recommends that you connect a VGA monitor to the appliance to monitor the conversion process, because the LOM connection might be lost during the conversion process.

With the cable attached, verify that the MPX appliance's components are functioning correctly. You are then ready to begin the conversion. The conversion process modifies the BIOS, installs the Citrix Hypervisor and a Management Service image, and copies the VPX image to the solid-state drive.

The conversion process sets up a redundant array of independent disks (RAID) controller for local storage:

- (SSD slot # 1 and SSD slot # 2)
- Citrix ADC VPX storage (SSD slot # 3 and SSD slot # 4)

After the conversion process, you modify the configuration of the appliance and apply a new license. You can then provision the VPX instances through the Management Service on what is now an SDX appliance.

To verify proper operation of the MPX appliance's components

1. Access the console port and enter the administrator credentials.
2. Run the following command from the command line interface of the appliance to display the serial number: `show hardware`

The serial number might be helpful in case you want to contact Citrix Technical Support.

Example

```
1 show hardware
2     Platform: NSMPX-14000 12*CPU+16*IX+2*E1K+2*CVM N3 250101
3     Manufactured on: 10/2/2015
4     CPU: 2600MHZ
5     Host Id: 234913926
6     Serial no: JSW4UCKKM5
7     Encoded serial no: JSW4UCKKM5
8 Done
9 <!--NeedCopy-->
```

3. Run the following command to display the status of the active 10G interfaces: `show interface`
4. In the `show interface` command's output, verify that all the interfaces are enabled and the status of every interface is shown as UP/UP.

Note: If you do not have an SFP+ transceiver for every port, verify the interfaces in stages. After checking the first set of interfaces, unplug the SFP+ transceivers and plug them in to the next set of ports.

5. Run the following command for each of the interfaces that are not in the UP/UP state:
`enable interface 10/x`
where x is the new interface number.
6. Run the following command to verify that the status of the power supplies is normal: `stat system -detail`
7. Run the following command to generate a tar of system configuration data and statistics: `show techsupport`

Note: The output of the command is available in the `/var/tmp/support/collector_<IP_address>_P_<date>.tar.gz` file. Copy this file to another computer for future

reference. The output of the command might be helpful in case you want to contact Citrix Technical Support.

- At the command line interface, switch to the shell prompt. Type: `shell`
- Run the following command to verify the number of Cavium cards available depending upon your appliance: `root@ns## grep "cavium"/var/nslog/dmesg.boot`

Example

```
1 root@ns# grep &quot;cavium&quot; /var/nslog/dmesg.boot
2 Cavium cavium_probe : found card 0x177d,device=0x11
3 cavium0 mem 0xdd600000-0xdd6ffffff irq 32 at device 0.0 on pci3
4 Cavium cavium_probe : found card 0x177d,device=0x11
5 cavium1 mem 0xfaa00000-0xfaaffffff irq 64 at device 0.0 on pci136
6 <!--NeedCopy-->
```

- Run the following command to verify the RAM memory reserved for shared memory depending upon your appliance: `root@ns## grep "memory"/var/nslog/dmesg.boot`

Example

```
1 root@ns# grep &quot;memory&quot; /var/nslog/dmesg.boot
2 real memory = 70866960384 (67584 MB)
3 avail memory = 66267971584 (63198 MB)
4 <!--NeedCopy-->
```

- Run the following command to verify the number of CPU cores depending upon your appliance: `root@ns## grep "cpu"/var/nslog/dmesg.boot`

Example

```
1 root@ns# grep &quot;cpu&quot; /var/nslog/dmesg.boot
2 cpu0 (BSP): APIC ID: 0
3 cpu1 (AP): APIC ID: 2
4 cpu2 (AP): APIC ID: 4
5 cpu3 (AP): APIC ID: 6
6 cpu4 (AP): APIC ID: 8
7 cpu5 (AP): APIC ID: 10
8 cpu6 (AP): APIC ID: 32
9 cpu7 (AP): APIC ID: 34
10 cpu8 (AP): APIC ID: 36
11 cpu9 (AP): APIC ID: 38
12 cpu10 (AP): APIC ID: 40
13 cpu11 (AP): APIC ID: 42
14 cpu0: &lt;ACPI CPU&gt; on acpi0
15 acpi_throttle0: &lt;ACPI CPU Throttling&gt; on cpu0
```

```

16 cpu1: &lt;ACPI CPU&gt; on acpi0
17 acpi_throttle1: &lt;ACPI CPU Throttling&gt; on cpu1
18 cpu2: &lt;ACPI CPU&gt; on acpi0
19 acpi_throttle2: &lt;ACPI CPU Throttling&gt; on cpu2
20 cpu3: &lt;ACPI CPU&gt; on acpi0
21 acpi_throttle3: &lt;ACPI CPU Throttling&gt; on cpu3
22 cpu4: &lt;ACPI CPU&gt; on acpi0
23 acpi_throttle4: &lt;ACPI CPU Throttling&gt; on cpu4
24 cpu5: &lt;ACPI CPU&gt; on acpi0
25 acpi_throttle5: &lt;ACPI CPU Throttling&gt; on cpu5
26 cpu6: &lt;ACPI CPU&gt; on acpi0
27 acpi_throttle6: &lt;ACPI CPU Throttling&gt; on cpu6
28 cpu7: &lt;ACPI CPU&gt; on acpi0
29 acpi_throttle7: &lt;ACPI CPU Throttling&gt; on cpu7
30 cpu8: &lt;ACPI CPU&gt; on acpi0
31 acpi_throttle8: &lt;ACPI CPU Throttling&gt; on cpu8
32 cpu9: &lt;ACPI CPU&gt; on acpi0
33 acpi_throttle9: &lt;ACPI CPU Throttling&gt; on cpu9
34 cpu10: &lt;ACPI CPU&gt; on acpi0
35 acpi_throttle10: &lt;ACPI CPU Throttling&gt; on cpu10
36 cpu11: &lt;ACPI CPU&gt; on acpi0
37 acpi_throttle11: &lt;ACPI CPU Throttling&gt; on cpu11
38 root@ns#
39 <!--NeedCopy-->

```

12. Run the following command to verify that the /var drive is mounted as /dev/ad8s1e: root@ns#
df -h
13. Run the ns_hw_err.bash script, which checks for latent hardware errors: root@ns##
ns_hw_err.bash

Example

```

1 root@ns# ns_hw_err.bash
2 NetScaler NS10.1: Build 133.11.nc, Date: Sep 21 2015, 17:59:51
3 platform: serial JSW4UCKKM5
4 platform: sysid 250101 - NSMPX-14000 12*CPU+16*IX+2*E1K+2*CVM N3
5 HDD MODEL: ar0: 227328MB &lt;Intel MatrixRAID RAID1&gt; status:
  READY
6 Generating the list of newslog files to be processed...
7 Generating the events from newslog files...
8 Checking for HDD errors...
9 Checking for HDD SMART errors...
10 Checking for Flash errors...
11 /var/nslog/dmesg.prev:* DEVELOPER mode - run NetScaler manually!
12 *****


```

```
13 FOUND          1 Flash errors: DEVELOPER mode - run NetScaler
    manually
14 *****
15 Checking for SSL errors...
16 Checking for BIOS errors...
17 Checking for SMB errors...
18 Checking for MotherBoard errors...
19 Checking for CMOS errors...
20          License year: 2015: OK
21 License server failed at startup. Check /var/log/license.log
22 Vendor daemon failed at startup. Check /var/log/license.log
23 Checking for SFP/NIC errors...
24 Checking for Firmware errors...
25 Checking for License errors...
26 Checking for Undetected CPUs...
27 Checking for DIMM flaps...
28 Checking for LOM errors...
29 Checking the Power Supply Errors...
30 root@ns#
31 <!--NeedCopy-->
```

14. Important: Physically disconnect all ports except the LOM port, including the management port, from the network.
15. At the shell prompt, switch to the Citrix ADC command line. Type: `exit`
16. Run the following command to shut down the appliance: `shutdown -p now`

To upgrade the appliance

1. Power off the Citrix ADC appliance.
2. Locate two solid-state drives (SSDs) on the back of the appliance in slot #1 and slot #2, as shown in the following figure:

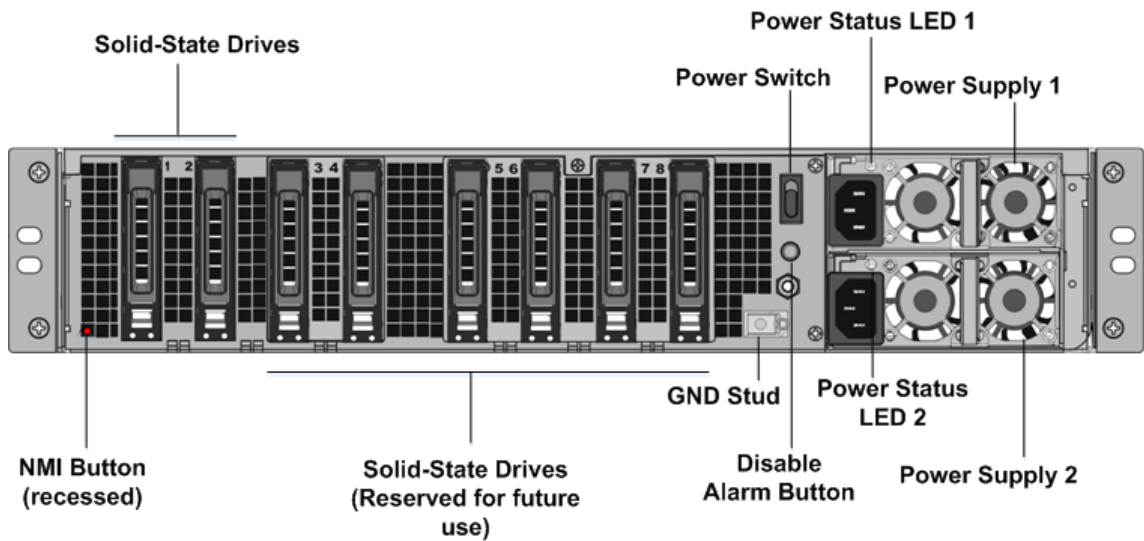

3. Verify that the replacement SSDs are the ones required for your Citrix ADC model. The conversion requires minimum of four SSDs. The Citrix label is on the top of one of the SSDs. The SSD is pre-populated with a new version of the BIOS and a recent build of the Management Service. This SSD must be installed in slot # 1.
4. Remove the SSDs by pushing the safety latch of the drive cover down while pulling the drive handle.
5. On the new Citrix certified SSD drive, open the drive handle completely to the left. Then insert the new drive into the slot #1 as far as possible.
6. To seat the drive, close the handle flush with the rear side of the appliance so that the drive locks securely into the slot.

Important: The orientation of the SSD is important. When you insert the drive, make sure that the Citrix product label is at the top.

7. Insert a second Citrix certified SSD, which matches the capacity of the SSD in slot #1, in slot # 2. Insert other blank Citrix certified SSDs in slots #3 and #4.

Note: If the license of your appliance is 14040, insert other blank Citrix certified SSDs in slots #3, #4, #5, and #6.

If the license of your appliance is 14060/14080/14100, insert other blank Citrix certified SSDs in slots #3, #4, #5, #6, #7, and #8.

Important: Mixing and matching of old and new SSDs is not supported. SSDs in slot #1 and slot # 2, which constitute the first RAID pair (local storage), must be of the same size and type. Similarly, SSDs in slot # 3 and slot # 4, which constitute the second RAID pair (VPX storage), must be of the same size and type. Only use drives that are part of the provided conversion kit.

8. Store the old SSDs for future handling.
9. Disconnect all network cables from the data ports and the management ports.

10. Start the Citrix ADC appliance. For instructions, see “Switching on the Appliance” in [Installing the hardware](#).

The conversion process can run for approximately 30 minutes, during which you must not power cycle the appliance. The entire conversion process might not be visible on the console and might appear to be unresponsive.

The conversion process updates the BIOS, installs the Citrix Hypervisor and the Management Service. It also copies the VPX image to the SSD for instance provisioning, and forms the Raid1 pair.

Note: The serial number of the appliance remains the same.

11. Keep the console cable attached during the conversion process. Allow the process to complete, at which point the netScaler-sdx login: prompt appears.
12. During the conversion process the LOM port connection might be lost as it resets the IP address to the default value of 192.168.1.3. The conversion status output is available on the VGA monitor.
13. To make sure that the conversion is successful, verify that the FVT result indicates success. Run the following command: `tail /var/log/fvt/fvt.log`

Example

```
1 [root@netScaler-sdx ~]# tail /var/log/fvt/fvt.log
2 Wed, 28 Oct 2015 04:40:47 /opt/xenSource/packages/files/fvt/workers/
  check_vf_count --pf_device="0000:89:00.1"; --vf_count=
  40;
3 Wed, 28 Oct 2015 04:40:47 => PASS
4 Wed, 28 Oct 2015 04:40:47 /opt/xenSource/packages/files/fvt/workers/
  check_vf_count --pf_device="0000:03:00.0"; --vf_count=
  8;
5 Wed, 28 Oct 2015 04:40:47 => PASS
6 Wed, 28 Oct 2015 04:40:47 /opt/xenSource/packages/files/fvt/workers/
  check_vf_count --pf_device="0000:88:00.0"; --vf_count=
  8;
7 Wed, 28 Oct 2015 04:40:47 => PASS
8 Wed, 28 Oct 2015 04:40:47 FVT RESULT: SUCCESS!<br />
9 [root@netScaler-sdx ~]#
10 <!--NeedCopy-->
```

To reconfigure the converted appliance

After the conversion process, the appliance no longer has its previous working configuration. Therefore, you can access the appliance through a web browser only by using the default IP address: 192.168.100.1/16. Configure a computer on network 192.168.0.0 and connect it directly to the appliance's management port (0/1) with a cross-over Ethernet cable. Alternately, access the SDX appliance

through a network hub by using a straight through Ethernet cable. Use the default credentials to log on, and then do the following:

1. Select the **Configuration** tab.
2. Verify that the System Resource section displays the accurate number of CPU cores, SSL cores, and the total memory for your SDX appliance.
3. Select the **System** node and, under **Set Up Appliance**, click **Network Configuration** to modify the IP address of the Management Service.
4. In the **Configure Network Configuration** dialog box, specify the following details:
 - Interface*—The interface through which clients connect to the Management Service. Possible values: 0/1, 0/2. Default: 0/1.
 - Citrix Hypervisor IP Address*—The IP address of Citrix Hypervisor.
 - Management Service IP Address*—The IP address of the Management Service.
 - Netmask*—The subnet mask for the subnet in which the SDX appliance is located.
 - Gateway*—The default gateway for the network.
 - DNS Server—The IP address of the DNS server.

*A mandatory parameter

5. Click OK. Connection to the Management Service is lost as the network information was changed.
6. Connect the SDX appliance's management port 0/1 to a switch to access it through the network. Browse to the IP address used earlier and log on with the default credentials.
7. Apply the new licenses. For instructions, see [SDX Licensing Overview](#).
8. Navigate to **Configuration > System** and, in the **System Administration** group, click **Reboot Appliance**. Click **Yes** to confirm. You are now ready to provision the VPX instances on the NetScaler SDX appliance. For instructions, see [Provisioning Citrix ADC Instances](#).

Convert a Citrix ADC MPX 14020 40G, MPX 14040 40G, MPX 14060 40G, MPX 14080 40G appliance to a Citrix ADC SDX 14020 40G, SDX 14040 40G, SDX 14060 40G, SDX 14080 40G appliance

August 11, 2020

You can convert a Citrix ADC MPX appliance to a NetScaler SDX appliance by upgrading the software through a new solid-state drive (SSD). Citrix supplies a field conversion kit to migrate a Citrix ADC MPX appliance to an SDX appliance.

The conversion requires minimum of four SSDs.

Note: Citrix recommends that you configure the lights out management (LOM) port of the appliance before starting the conversion process. For more information on the LOM port of the NetScaler appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

To convert an MPX appliance to an SDX appliance, you must access the appliance through a console cable attached to a computer or terminal. Before connecting the console cable, configure the computer or terminal to support the following configuration:

- VT100 terminal emulation
- 9600 baud
- 8 data bits
- 1 stop bit
- Parity and flow control set to NONE

Connect one end of the console cable to the RS232 serial port on the appliance, and the other end to the computer or terminal.

Note: To use a cable with an RJ-45 converter, insert the optional converter into the console port and attach the cable to it.

Citrix recommends you to connect a VGA monitor to the appliance to monitor the conversion process, because the LOM connection is lost during the conversion process.

With the cable attached, verify that the MPX appliance's components are functioning correctly. You are then ready to begin the conversion. The conversion process modifies the BIOS, installs a Citrix Hypervisor and a Service Virtual Machine image, and copies the NetScaler VPX image to the Solid State Drive.

The conversion process also sets up a redundant array of independent disks (RAID) controller for local storage (SSD slot # 1 and SSD slot # 2) and NetScaler VPX storage (SSD slot # 3 and SSD slot # 4).

After the conversion process, make modifications to the appliance's configuration and apply a new license. You can then provision the VPX instances through the Management Service on what is now a NetScaler SDX appliance.

Verify proper operation of the MPX appliance's components

1. Access the console port and enter the administrator credentials.
2. Run the following command from the command line interface of the appliance to display the serial number: `show hardware`

Example

```
1 show hardware
```



```

2      Platform: NSMPX-14000-40G 12*CPU+16*F1X+4*F4X+2*E1K+2*CVM N3
      250140
3      Manufactured on: 3/21/2016
4      CPU: 2600MHZ
5      Host Id: 234913926
6      Serial no: KZCHGCN810
7      Encoded serial no: KZCHGCN810
8 Done
9 <!--NeedCopy-->

```

The serial number might be helpful when you want to contact Citrix Technical Support.

3. Run the following command to display the status of the active interfaces:

show interface

Example

```

1 show interface
2 1)      Interface 0/1 (Gig Ethernet 10/100/1000 Mbits) #10
3          flags=0xc020 &lt;ENABLED, UP, UP, autoneg, HAMON, 802.1q&gt;
4          MTU=1500, native vlan=1, MAC=0c:c4:7a:41:ea:94, uptime 43
           h59m55s
5          Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
6              throughput 0
7          Actual: media UTP, speed 1000, duplex FULL, fctl OFF,
           throughput 1000
8          LLDP Mode: NONE
9          RX: Pkts(44337150) Bytes(2767558041) Errs(0) Drops(41260552)
           Stalls(0)
10         TX: Pkts(128116) Bytes(9004699) Errs(0) Drops(0) Stalls(0)
11         NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
12         Bandwidth thresholds are not set.
13 2)      Interface 0/2 (Gig Ethernet 10/100/1000 Mbits) #11
14         flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
           ;
15         MTU=1500, native vlan=1, MAC=0c:c4:7a:41:ea:95, downtime 44
           h00m08s
16         Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
17             throughput 0
18         LLDP Mode: NONE
19         RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
20         TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
21         NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
22         Bandwidth thresholds are not set.
23 3)      Interface 10/1 (10G Ethernet) #17

```

```
24     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
25     ;
26     MTU=1500, native vlan=1, MAC=68:05:ca:30:e1:40, downtime 44
27     h00m08s
28     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
29     throughput 0
30     LLDP Mode: NONE
31     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
32     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
33     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
34     Bandwidth thresholds are not set.
35 4) Interface 10/2 (10G Ethernet) #18
36     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
37     ;
38     MTU=1500, native vlan=1, MAC=68:05:ca:30:e1:41, downtime 44
39     h00m08s
40     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
41     throughput 0
42     LLDP Mode: NONE
43     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
44     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
45     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
46     Bandwidth thresholds are not set.
47 5) Interface 10/3 (10G Ethernet) #19
48     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
49     ;
50     MTU=1500, native vlan=1, MAC=68:05:ca:30:e1:42, downtime 44
51     h00m08s
52     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
53     throughput 0
54     LLDP Mode: NONE
55     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
56     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
57     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
58     Bandwidth thresholds are not set.
59 6) Interface 10/4 (10G Ethernet) #20
60     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
61     ;
62     MTU=1500, native vlan=1, MAC=68:05:ca:30:e1:43, downtime 44
63     h00m08s
64     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
65     throughput 0
66     LLDP Mode: NONE
67     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
68     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
```

```
61     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
62     Bandwidth thresholds are not set.
63 7)   Interface 10/5 (10G Ethernet) #13
64     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
65     ;
66     MTU=1500, native vlan=1, MAC=68:05:ca:2e:6b:a0, downtime 44
67     h00m08s
68     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
69     throughput 0
70     LLDP Mode: NONE
71     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
72     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
73     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
74     Bandwidth thresholds are not set.
75 8)   Interface 10/6 (10G Ethernet) #14
76     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
77     ;
78     MTU=1500, native vlan=1, MAC=68:05:ca:2e:6b:a1, downtime 44
79     h00m08s
80     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
81     throughput 0
82     LLDP Mode: NONE
83     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
84     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
85     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
86     Bandwidth thresholds are not set.
87 9)   Interface 10/7 (10G Ethernet) #15
88     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
89     ;
90     MTU=1500, native vlan=1, MAC=68:05:ca:2e:6b:a2, downtime 44
91     h00m08s
92     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
93     throughput 0
94     LLDP Mode: NONE
95     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
96     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
97     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
98     Bandwidth thresholds are not set.
99 10)  Interface 10/8 (10G Ethernet) #16
100    flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
101    ;
102    MTU=1500, native vlan=1, MAC=68:05:ca:2e:6b:a3, downtime 44
103    h00m08s
104    Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
105    throughput 0
106    LLDP Mode: NONE
```

```
 99      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
100      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
101      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
102      Bandwidth thresholds are not set.
103 11)   Interface 10/9 (10G Ethernet) #0
104      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
105      MTU=1500, native vlan=1, MAC=68:05:ca:30:e1:a0, downtime 44
106          h00m08s
107      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
108          throughput 0
109      LLDP Mode: NONE
110      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
111      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
112      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
113      Bandwidth thresholds are not set.
114 12)   Interface 10/10 (10G Ethernet) #1
115      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
116          ;
117      MTU=1500, native vlan=1, MAC=68:05:ca:30:e1:a1, downtime 44
118          h00m08s
119      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
120          throughput 0
121      LLDP Mode: NONE
122      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
123      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
124      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
125      Bandwidth thresholds are not set.
126 13)   Interface 10/11 (10G Ethernet) #2
127      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
128          ;
129      MTU=1500, native vlan=1, MAC=68:05:ca:30:e1:a2, downtime 44
130          h00m08s
131      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
132          throughput 0
133      LLDP Mode: NONE
134      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
135      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
136      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
137      Bandwidth thresholds are not set.
138 14)   Interface 10/12 (10G Ethernet) #3
139      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&gt;
140          ;
141      MTU=1500, native vlan=1, MAC=68:05:ca:30:e1:a3, downtime 44
142          h00m08s
143      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
```

```
137         throughput 0
138     LLDP Mode: NONE
139
140     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
141     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
142     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
143     Bandwidth thresholds are not set.
144
145 15)   Interface 10/13 (10G Ethernet) #4
146     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&
147         gt;
148     MTU=1500, native vlan=1, MAC=68:05:ca:30:e2:70, downtime 44
149         h00m08s
150     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
151         throughput 0
152     LLDP Mode: NONE
153     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
154     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
155     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
156     Bandwidth thresholds are not set.
157 16)   Interface 10/14 (10G Ethernet) #5
158     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&
159         gt;
160     MTU=1500, native vlan=1, MAC=68:05:ca:30:e2:71, downtime 44
161         h00m15s
162     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
163         throughput 0
164     LLDP Mode: NONE
165     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
166     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
167     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
168     Bandwidth thresholds are not set.
169 17)   Interface 10/15 (10G Ethernet) #6
170     flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&
171         gt;
172     MTU=1500, native vlan=1, MAC=68:05:ca:30:e2:72, downtime 44
173         h00m15s
174     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
175         throughput 0
176     LLDP Mode: NONE
177     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
178     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
179     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
180     Bandwidth thresholds are not set.
181 18)   Interface 10/16 (10G Ethernet) #7
```

```
176      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&
177      >;
177      MTU=1500, native vlan=1, MAC=68:05:ca:30:e2:73, downtime 44
178      h00m15s
178      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
179      throughput 0
180      LLDP Mode: NONE
181
182      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
183      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
184      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
185      Bandwidth thresholds are not set.
186  19)  Interface 40/1 (40G Ethernet) #9
187      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&
188      >;
188      MTU=1500, native vlan=1, MAC=3c:fd:fe:9c:f9:98, downtime 44
189      h00m15s
189      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
190      throughput 0
191      LLDP Mode: NONE
192      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
193      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
194      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
195      Bandwidth thresholds are not set.
196  20)  Interface 40/2 (40G Ethernet) #21
197      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&
198      >;
198      MTU=1500, native vlan=1, MAC=3c:fd:fe:9c:fa:68, downtime 44
199      h00m15s
199      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
200      throughput 0
201      LLDP Mode: NONE
202      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
203      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
204      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
205      Bandwidth thresholds are not set.
206  21)  Interface 40/3 (40G Ethernet) #12
207      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&
208      >;
208      MTU=1500, native vlan=1, MAC=3c:fd:fe:9c:f9:f8, downtime 44
209      h00m15s
209      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
210      throughput 0
211      LLDP Mode: NONE
212      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
```

```

213      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
214      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
215      Bandwidth thresholds are not set.
216  22)  Interface 40/4 (40G Ethernet) #8
217      flags=0x4000 &lt;ENABLED, DOWN, down, autoneg, HAMON, 802.1q&
          gt;
218      MTU=1500, native vlan=1, MAC=3c:fd:fe:9c:f9:e0, downtime 44
          h00m15s
219      Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
220      throughput 0
221      LLDP Mode: NONE
222      RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
223      TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
224      NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
225      Bandwidth thresholds are not set.
226  23)  Interface LO/1 (Netscaler Loopback interface) #22
227      flags=0x20008020 &lt;ENABLED, UP, UP&gt;
228      MTU=1500, native vlan=1, MAC=0c:c4:7a:41:ea:94, uptime 44
          h00m15s
229      LLDP Mode: NONE
230      RX: Pkts(103847611) Bytes(14441166499) Errs(0) Drops(0) Stalls
          (0)
231      TX: Pkts(206723664) Bytes(20488047637) Errs(0) Drops(0) Stalls
          (0)
232      Bandwidth thresholds are not set.
233      Done
234      <!--NeedCopy-->

```

4. In the show interface command's output, verify that all of the interfaces are enabled and the status of every interface is shown as UP/UP.

Notes:

- The interface status is displayed as UP/UP only if the cables are connected to the interfaces.
- If you do not have an SFP+ transceiver for every port, verify the interfaces in stages. After checking the first set of interfaces, unplug the SFP+ transceivers and plug them in to the next set of ports.

5. Run the following command for each of the interfaces that are not in the UP/UP state:

```

1  enable interface 10/x
2  enable interface 40/x
3  <!--NeedCopy-->

```

Where x is the new interface number.

Example:

```
1 enable interface 10/1
2 Done
3 &gt; enable interface 40/1
4 Done
5 <!--NeedCopy-->
```

6. Run the following command to verify that the status of the power supplies is normal: stat system -detail

Example

```
1 stat system -detail
2 NetScaler Executive View
3 System Information:
4 Up since Mon Mar 21 13:53:22 2016
5 Memory usage (MB) 1177
6 InUse Memory (%) 5.37
7 Number of CPUs 7
8 System Health Statistics (Standard):
9 CPU 0 Core Voltage (Volts) 0.99
10 CPU 1 Core Voltage (Volts) 0.98
11 Main 3.3 V Supply Voltage 3.36
12 Standby 3.3 V Supply Voltage 3.31
13 +5.0 V Supply Voltage 5.06
14 +12.0 V Supply Voltage 12.08
15 Battery Voltage (Volts) 3.17
16 Intel CPU Vtt Power(Volts) 1.01
17 5V Standby Voltage(Volts) 0.00
18 Voltage Sensor2(Volts) 0.00
19 CPU Fan 0 Speed (RPM) 4650
20 CPU Fan 1 Speed (RPM) 4575
21 System Fan Speed (RPM) 4650
22 System Fan 1 Speed (RPM) 4650
23 System Fan 2 Speed (RPM) 4650
24 CPU 0 Temperature (Celsius) 42
25 CPU 1 Temperature (Celsius) 49
26 Internal Temperature (Celsius) 36
27 Power supply 1 status NORMAL
28 Power supply 2 status NORMAL
29 Power supply 3 status NOT SUPPORTED
30 Power supply 4 status NOT SUPPORTED
31 System Disk Statistics:
32 /flash Size (MB) 16858
33 /flash Used (MB) 186
```



```
34 /flash Available (MB) 15323
35 /flash Used (%) 1
36 /var Size (MB) 143802
37 /var Used (MB) 781
38 /var Available (MB) 131517
39 /var Used (%) 0
40 System Health Statistics(Auxiliary):
41 Voltage 0 (Volts) 1.49
42 Voltage 1 (Volts) 1.49
43 Voltage 2 (Volts) 1.50
44 Voltage 3 (Volts) 1.49
45 Voltage 4 (Volts) 1.49
46 Voltage 5 (Volts) 0.00
47 Voltage 6 (Volts) 0.00
48 Voltage 7 (Volts) 0.00
49 Fan 0 Speed (RPM) 4650
50 Fan 1 Speed (RPM) 0
51 Fan 2 Speed (RPM) 0
52 Fan 3 Speed (RPM) 0
53 Temperature 0 (Celsius) 28
54 Temperature 1 (Celsius) 43
55 Temperature 2 (Celsius) 0
56 Temperature 3 (Celsius) 0
57 Done
58 <!--NeedCopy-->
```

7. Run the following command to generate a tar of system configuration data and statistics: `show techsupport`

Example

```
1 show techsupport
2 showtechsupport data collector tool - $Revision: #2 $!
3 NetScaler version 10.5
4 Creating /var/tmp/support ....
5 The NS IP of this box is 192.168.100.1
6 Current HA state: Primary (or this is not part of HA pair!)
7 All the data will be collected under
8     /var/tmp/support/collector_P_192.168.100.1_23Mar2016_10_00
9 Copying selected configuration files from nsconfig ....
10 Copying WebInterface configuration files (if WI is installed) ....
11     .... WI is not installed on this system. Nothing to copy.
12 Running shell commands ....
13 Running CLI show commands ....
14 Running CLI stat commands ....
```

```
15  Running vtysh commands ....
16  Determining newslog files to archive ....
17      Last newslog file index=1
18      Warning! Missing newslog.0 and newslog.0.tar and newslog.0.
        tar.gz file!
19      Warning! Missing newslog.199 and newslog.199.tar and
        newslog.199.tar.gz file!
20      Warning! Missing newslog.198 and newslog.198.tar and
        newslog.198.tar.gz file!
21      Warning! Missing newslog.197 and newslog.197.tar and
        newslog.197.tar.gz file!
22      Warning! Missing newslog.196 and newslog.196.tar and
        newslog.196.tar.gz file!
23      Five newslog files missing
24
25      .... copied 2 files from this directory.
26  Copying core files from /var/core .... (last 5 files created within
        the last week)
27      .... Nothing to copy .... No files created within the last one
        week
28  Copying core files from /var/crash .... (last 5 files created within
        the last week)
29      .... Nothing to copy .... No files created within the last one
        week
30  Copying imported files and mapping files ....
31  Copying GSLB location database files ....
32  Copying files from /var/log/db ....
33  Copying messages,ns.log,dmesg and other log files ....
34  Warning : cluster showtech node failure log file: /var/tmp/support/
        collector_P_192.168.100.1_23Mar2016_10_00/
        cluster_showtech_node_failure.log is not present
35  Archiving all the data into &quot;/var/tmp/support/collector_P_192
        .168.100.1_23Mar2016_10_00.tar.gz&quot; ....
36  Created a symbolic link for the archive with /var/tmp/support/support.
        tgz
37  /var/tmp/support/support.tgz ---- points to ---&gt; /var/tmp/support/
        collector_P_192.168.100.1_23Mar2016_10_00.tar.gz
38  If this node is part of HA pair, please run it on the other node also
        !!
39  Done
40  <!--NeedCopy-->
```

Note: The output of the command is available in the /var/tmp/support/collector_<IP_address>_P_<date>.tar.gz file. Copy this file to another computer for future reference. The output of the command might be

helpful when you want to contact Citrix Technical Support.

8. At the command line interface, switch to the shell prompt. Type: `shell`

Example

```
1 shell
2 Copyright (c) 1992-2013 The FreeBSD Project.
3 Copyright (c) 1979, 1980, 1983, 1986, 1988, 1989, 1991, 1992, 1993,
   1994
4     The Regents of the University of California. All rights
   reserved.
5 <!--NeedCopy-->
```

9. Run the following command to verify the number of Cavium cards available depending upon your appliance:

```
root@ns## grep "cavium"/var/nslog/dmesg.boot
```

Example

```
1 /var/nslog/dmesg.boot
2 Cavium cavium_probe : found card 0x177d,device=0x11
3 cavium0 mem 0xde200000-0xde2ffffff irq 32 at device 0.0 on pci3
4 cavium0: [ITHREAD]
5 Cavium cavium_probe : found card 0x177d,device=0x11
6 cavium1 mem 0xfb400000-0xfb4ffffff irq 64 at device 0.0 on pci136
7 cavium1: [ITHREAD]
8 Cavium cavium_probe : found card 0x177d,device=0x11
9 cavium0 mem 0xde200000-0xde2ffffff irq 32 at device 0.0 on pci3
10 cavium0: [ITHREAD]
11 Cavium cavium_probe : found card 0x177d,device=0x11
12 cavium1 mem 0xfb400000-0xfb4ffffff irq 64 at device 0.0 on pci136
13 cavium1: [ITHREAD]
14 root@ns#
15 <!--NeedCopy-->
```

10. Run the following command to verify the RAM memory reserved for shared memory depending upon your appliance:

```
root@ns# grep "memory" /var/nslog/dmesg.boot
```

Example

```
1 /var/nslog/dmesg.boot
2 real memory = 70866960384 (67584 MB)
3 avail memory = 66206515200 (63139 MB)
```

```
4 NS-KERN map_shared_mem_ioctl (cpu 11, NSPPE-00): Reserving 596 MB for
   shared memory type 0
5 real memory = 70866960384 (67584 MB)
6 avail memory = 66206515200 (63139 MB)
7 root@ns#
8 <!--NeedCopy-->
```

11. Run the following command to verify the number of CPU cores depending upon your appliance:

```
root@ns## grep "cpu"/var/nslog/dmesg.boot
```

Example

```
1 root@ns# grep "cpu" /var/nslog/dmesg.boot
2 cpu0 (BSP): APIC ID: 0
3 cpu1 (AP): APIC ID: 2
4 cpu2 (AP): APIC ID: 4
5 cpu3 (AP): APIC ID: 6
6 cpu4 (AP): APIC ID: 8
7 cpu5 (AP): APIC ID: 10
8 cpu6 (AP): APIC ID: 32
9 cpu7 (AP): APIC ID: 34
10 cpu8 (AP): APIC ID: 36
11 cpu9 (AP): APIC ID: 38
12 cpu10 (AP): APIC ID: 40
13 cpu11 (AP): APIC ID: 42
14 cpu0: <ACPI CPU> on acpi0
15 cpu1: <ACPI CPU> on acpi0
16 cpu2: <ACPI CPU> on acpi0
17 cpu3: <ACPI CPU> on acpi0
18 cpu4: <ACPI CPU> on acpi0
19 cpu5: <ACPI CPU> on acpi0
20 cpu6: <ACPI CPU> on acpi0
21 cpu7: <ACPI CPU> on acpi0
22 cpu8: <ACPI CPU> on acpi0
23 cpu9: <ACPI CPU> on acpi0
24 cpu10: <ACPI CPU> on acpi0
25 cpu11: <ACPI CPU> on acpi0
26 est0: <Enhanced SpeedStep Frequency Control> on cpu0
27 p4tcc0: <CPU Frequency Thermal Control> on cpu0
28 est1: <Enhanced SpeedStep Frequency Control> on cpu1
29 p4tcc1: <CPU Frequency Thermal Control> on cpu1
30 est2: <Enhanced SpeedStep Frequency Control> on cpu2
31 p4tcc2: <CPU Frequency Thermal Control> on cpu2
32 est3: <Enhanced SpeedStep Frequency Control> on cpu3
33 p4tcc3: <CPU Frequency Thermal Control> on cpu3
```

```
34 est4: <Enhanced SpeedStep Frequency Control> on cpu4
35 p4tcc4: <CPU Frequency Thermal Control> on cpu4
36 est5: <Enhanced SpeedStep Frequency Control> on cpu5
37 p4tcc5: <CPU Frequency Thermal Control> on cpu5
38 est6: <Enhanced SpeedStep Frequency Control> on cpu6
39 p4tcc6: <CPU Frequency Thermal Control> on cpu6
40 est7: <Enhanced SpeedStep Frequency Control> on cpu7
41 p4tcc7: <CPU Frequency Thermal Control> on cpu7
42 est8: <Enhanced SpeedStep Frequency Control> on cpu8
43 p4tcc8: <CPU Frequency Thermal Control> on cpu8
44 est9: <Enhanced SpeedStep Frequency Control> on cpu9
45 p4tcc9: <CPU Frequency Thermal Control> on cpu9
46 est10: <Enhanced SpeedStep Frequency Control> on cpu10
47 p4tcc10: <CPU Frequency Thermal Control> on cpu10
48 est11: <Enhanced SpeedStep Frequency Control> on cpu11
49 p4tcc11: <CPU Frequency Thermal Control> on cpu11
50 NS-KERN map_shared_mem_ioctl (cpu 11, NSPPE-00): Reserving 596 MB for
    shared memory type 0
51 cpu0 (BSP): APIC ID: 0
52 cpu1 (AP): APIC ID: 2
53 cpu2 (AP): APIC ID: 4
54 cpu3 (AP): APIC ID: 6
55 cpu4 (AP): APIC ID: 8
56 cpu5 (AP): APIC ID: 10
57 cpu6 (AP): APIC ID: 32
58 cpu7 (AP): APIC ID: 34
59 cpu8 (AP): APIC ID: 36
60 cpu9 (AP): APIC ID: 38
61 cpu10 (AP): APIC ID: 40
62 cpu11 (AP): APIC ID: 42
63 cpu0: <ACPI CPU> on acpi0
64 cpu1: <ACPI CPU> on acpi0
65 cpu2: <ACPI CPU> on acpi0
66 cpu3: <ACPI CPU> on acpi0
67 cpu4: <ACPI CPU> on acpi0
68 cpu5: <ACPI CPU> on acpi0
69 cpu6: <ACPI CPU> on acpi0
70 cpu7: <ACPI CPU> on acpi0
71 cpu8: <ACPI CPU> on acpi0
72 cpu9: <ACPI CPU> on acpi0
73 cpu10: <ACPI CPU> on acpi0
74 cpu11: <ACPI CPU> on acpi0
75 est0: <Enhanced SpeedStep Frequency Control> on cpu0
76 p4tcc0: <CPU Frequency Thermal Control> on cpu0
77 est1: <Enhanced SpeedStep Frequency Control> on cpu1
```

```

78 p4tcc1: &lt;CPU Frequency Thermal Control&gt; on cpu1
79 est2: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu2
80 p4tcc2: &lt;CPU Frequency Thermal Control&gt; on cpu2
81 est3: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu3
82 p4tcc3: &lt;CPU Frequency Thermal Control&gt; on cpu3
83 est4: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu4
84 p4tcc4: &lt;CPU Frequency Thermal Control&gt; on cpu4
85 est5: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu5
86 p4tcc5: &lt;CPU Frequency Thermal Control&gt; on cpu5
87 est6: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu6
88 p4tcc6: &lt;CPU Frequency Thermal Control&gt; on cpu6
89 est7: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu7
90 p4tcc7: &lt;CPU Frequency Thermal Control&gt; on cpu7
91 est8: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu8
92 p4tcc8: &lt;CPU Frequency Thermal Control&gt; on cpu8
93 est9: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu9
94 p4tcc9: &lt;CPU Frequency Thermal Control&gt; on cpu9
95 est10: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu10
96 p4tcc10: &lt;CPU Frequency Thermal Control&gt; on cpu10
97 est11: &lt;Enhanced SpeedStep Frequency Control&gt; on cpu11
98 p4tcc11: &lt;CPU Frequency Thermal Control&gt; on cpu11
99 root@ns#
100 <!--NeedCopy-->

```

12. Run the following command to verify that the /var drive is mounted as /dev/ ar0s1a: root@ns# df -h

Example

```

1 root@ns# df -h
2 Filesystem      Size   Used  Avail Capacity  Mounted on
3 /dev/md0        327M   317M    3.1M    99%      /
4 devfs           1.0k   1.0k     0B   100%    /dev
5 procfs          4.0k   4.0k     0B   100%    /proc
6 /dev/ar0s1a     16G    186M    15G     1%    /flash
7 /dev/ar0s1e    140G   857M   128G     1%    /var
8 root@ns#
9 <!--NeedCopy-->

```

13. Type the following command to run the ns_hw_err.bash script, which checks for latent hardware errors: root@ns# ns_hw_err.bash

Example

```

1 root@ns# ns_hw_err.bash
2 NetScaler NS10.5: Build 59.71.nc, Date: Mar  2 2016, 05:22:19

```

```
3 platform: serial KZCHGCN810
4 platform: sysid 250140 - NSMPX-14000-40G 12*CPU+16*F1X+4*F4X+2*E1K+2*
  CVM N3
5 HDD MODEL: ar0: 227328MB &lt;Intel MatrixRAID RAID1&gt;; status: READY
6
7 Generating the list of newslog files to be processed...
8 Generating the events from newslog files...
9 Checking for HDD errors...
10 Checking for HDD SMART errors...
11 Checking for Flash errors...
12 /var/nslog/dmesg.boot:* DEVELOPER mode - run NetScaler manually! *
13 /var/tmp/ns_hw_tmp_10831//dmesg-a.out:* DEVELOPER mode - run NetScaler
  manually! *
14 *****
15 FOUND          2 Flash errors: DEVELOPER mode - run NetScaler manually
16 *****
17 Checking for Mega Raid Controller errors...
18 Checking for SSL errors...
19 Checking for BIOS errors...
20 Checking for SMB errors...
21 Checking for MotherBoard errors...
22 Checking for CMOS errors...
23     License year: 2016: OK
24 License server failed at startup. Check /var/log/license.log
25 Vendor daemon failed at startup. Check /var/log/license.log
26 Checking for SFP/NIC errors...
27 Checking for Firmware errors...
28 Checking for License errors...
29 Checking for Undetected CPUs...
30 Checking for DIMM flaps...
31 Checking for LOM errors...
32 Checking the Power Supply Errors...
33 root@ns#
34 <!--NeedCopy-->
```

14. **Important:** Physically disconnect all ports except the LOM port, including the management port, from the network.

15. At the shell prompt, switch to the NetScaler command line. Type: exit

Example

```
1 root@ns# exit
2 logout
3 Done
4 <!--NeedCopy-->
```

16. Run the following command to shut down the appliance. You are asked if you want to completely stop the NetScaler. Type: `shutdown -p now`


Example

```
1 root@ns#
2 root@ns# exit
3 logout
4 Done
5 <!--NeedCopy-->
```

Upgrade the appliance

To upgrade the appliance, follow these steps:

1. Power off the NetScaler appliance.
2. Locate two solid-state drives (SSDs) on the back of the appliance in slot #1 and slot #2, as shown in the following figure:

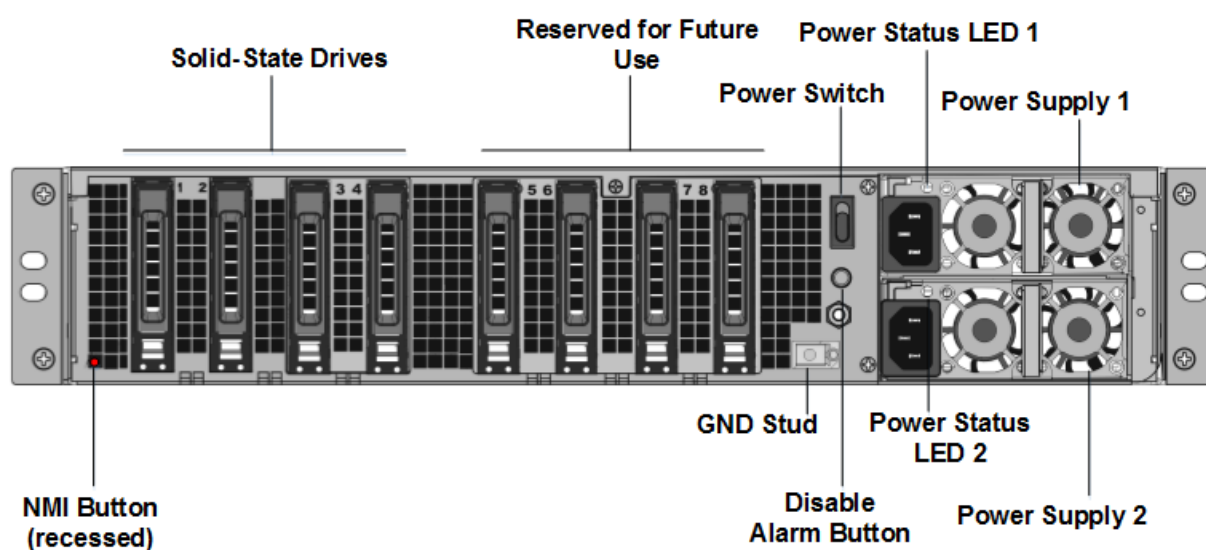

3. Verify that the replacement solid-state drives (SSDs) are the ones required for your NetScaler model. The conversion requires minimum of four SSDs. The Citrix label is on the top of one of the solid-state drives, which is pre-populated with a new version of BIOS and a recent build of the required NetScaler SDX Management Service. This SSD must be installed in slot # 1.
4. Remove the SSDs by pushing the safety latch of the drive cover down while pulling the drive handle.
5. On the new Citrix Certified SSD drive, open the drive handle completely to the left, and then insert the new drive into the slot #1 as far as possible.

6. To seat the drive, close the handle flush with the rear side of the appliance so that the drive locks securely into the slot.

Important: The orientation of the SSD is important. When you insert the drive, make sure that the Citrix product label is at the side.

7. Insert a second Citrix certified SSD, which matches the capacity of the SSD in slot #1, in slot # 2.

Note: If the license of your appliance is 14040 40G, 14060 40G, 14080 40G, insert more blank Citrix certified SSDs in slots #3, #4, #5, and #6.

NetScaler SDX Model	Included Virtual Instances	Platform Maximum	SSDs included on base model	Extra SSDs for max instances
SDX 14020 40G	5	25	Two 240 GB; Two 300 GB	Two 300 GB
SDX 14040 40G, SDX 14060 40G, SDX 14080 40G	25	25	Two 240 GB; Four 300 GB	N/A

Important: Mixing and matching of old and new SSDs is not supported. SSDs in slot #1 and slot #2, which constitute the first RAID pair (local storage), must be of the same size and type. Similarly, SSDs in slot #3 and slot #4, which constitute the second RAID pair (VPX storage), must be of the same size and type. Use only drives that are part of the provided conversion kit.

8. Disconnect all network cables from the data ports and the management ports.

9. Start the NetScaler appliance. For instructions, see “Switching on the Appliance” in Installing the Hardware.

The conversion process can run for approximately 30 minutes, during which you must not power cycle the appliance. The entire conversion process might not be visible on the console and might appear to be unresponsive.

The conversion process updates the BIOS, installs the Citrix Hypervisor and the Management Service Operating system, and copies the NetScaler VPX image to the SSD for instance provisioning, and forms the Raid1 pair.

Note: The serial number of the appliance remains the same.

10. Keep the console cable attached during the conversion process. Allow the process to complete, at which point the netscaler-sdx login: prompt appears.

11. During the conversion process the LOM port connection might be lost as it resets the IP address to the default value of 192.168.1.3. The conversion status output is available on the VGA monitor.

12. The default credentials are now changed from nsroot/nsroot to root/nsroot once the appliance is converted from an MPX to SDX.

13. To make sure that the conversion is successful, verify that the FVT result indicates success. Run the following command: `tail /var/log/fvt/fvt.log`

Reconfigure the converted appliance

After the conversion process, the appliance no longer has its previous working configuration. Therefore, you can access the appliance through a web browser only by using the default IP address: 192.168.100.1/16. Configure a computer on network 192.168.0.0 and connect it directly to the appliance's management port (0/1) with a cross-over Ethernet cable, or access the NetScaler SDX appliance through a network hub by using a straight through Ethernet cable. Use the default credentials to log on, and then do the following:

1. Select the Configuration tab.
2. Verify that the System Resource section displays the accurate number of CPU cores, SSL cores, and the total memory for your NetScaler SDX appliance.
3. Select the **System** node and, under **Set Up Appliance**, click **Network Configuration** to modify network information of the Management Service.
4. In the **Modify Network Configuration** dialog box, specify the following details:
 - Interface*—The interface through which clients connect to the Management Service. Possible values: 0/1, 0/2. Default: 0/1.
 - Citrix Hypervisor IP Address*—The IP address of Citrix Hypervisor.
 - Management Service IP Address*—The IP address of the Management Service.
 - Netmask*—The subnet mask for the subnet in which the SDX appliance is located.
 - Gateway*—The default gateway for the network.
 - DNS Server—The IP address of the DNS server.

*A mandatory parameter

1. Click OK. Connection to the Management Service is lost as the network information was changed.
2. Connect the NetScaler SDX appliance's management port 0/1 to a switch to access it through the network. Browse to the IP address used earlier and log on with the default credentials.
3. Apply the new licenses. For instructions, see [SDX Licensing Overview](#).
4. Navigate to **Configuration > System** and, in the **System Administration** group, click **Reboot Appliance**. Click **Yes** to confirm. You are now ready to provision the VPX instances on the NetScaler SDX appliance. For instructions, see [Provisioning Citrix ADC instances](#).

Convert a Citrix ADC MPX 8900 appliance to a Citrix ADC SDX 8900 appliance

August 18, 2020

You can convert a Citrix ADC MPX appliance to a Citrix ADC SDX appliance by upgrading the software through a new solid-state drive (SSD). Citrix supplies a field conversion kit to migrate a Citrix ADC MPX appliance to a Citrix ADC SDX appliance.

Note

Citrix recommends that you configure the lights out management (LOM) port of the Citrix ADC appliance before starting the conversion process. For more information on the LOM port of the Citrix ADC appliance, see

[Lights out management port of the Citrix ADC appliance.](#)

To convert a Citrix ADC MPX appliance to a Citrix ADC SDX appliance, you must access the appliance through a console cable attached to a computer or terminal. Before connecting the console cable, configure the computer or terminal to support the following configuration:

- VT100 terminal emulation
- 9600 baud
- 8 data bits
- 1 stop bit
- Parity and flow control set to NONE

Connect one end of the console cable to the RS232 serial port on the appliance, and the other end to the computer or terminal.

Note


To use a cable with an RJ-45 converter, insert the optional converter into the console port and attach the cable to it.

With the cable attached, verify that the MPX appliance's components are functioning correctly. You are then ready to begin the conversion. The conversion process modifies the BIOS, installs a Citrix Hypervisor and a Service Virtual Machine image, and copies the Citrix ADC VPX image to the SSD.

After the conversion process, you modify the appliance's configuration and apply a new license. You can then provision the VPX instances through the Management Service on what is now a Citrix ADC SDX appliance.

The following figure shows the front panel of the MPX 89xx.

Figure 1. Citrix ADC MPX 89xx front panel

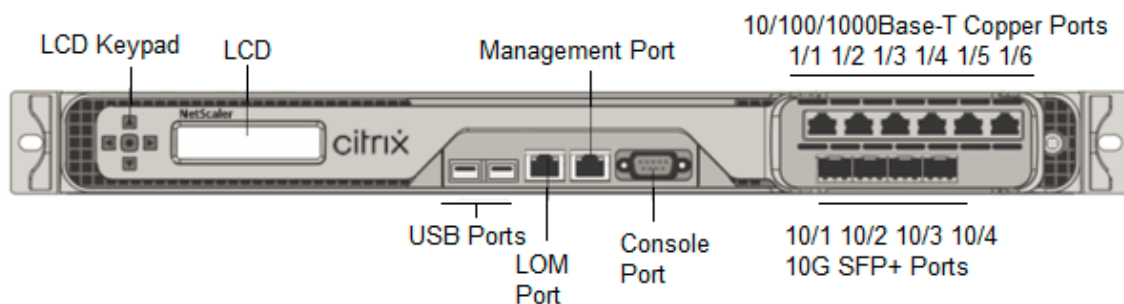

To verify proper operation of the MPX appliance's components

1. Access the console port and enter the administrator credentials.
2. Run the following command from the command line interface of the appliance to display the serial number: **show hardware**

The serial number might be helpful in case you want to contact Citrix Technical Support.

Example

```

1 > show hardware
2 Platform: NSMPX-8900 8*CPU+4*F1X+6*E1K+1*E1K+1*COL 8955 30010
3 Manufactured on: 12/3/2018
4 CPU: 2100MHZ
5 Host Id: 1862303878
6 Serial no: JVFUJCZT1E
7 Encoded serial no: JVFUJCZT1E
8 BMC Revision: 4.51
9 Done
10 <!--NeedCopy-->

```

3. Run the following command to display the status of the active 1G and 10G interfaces: **show interface**
4. In the show interface command's output, verify that all the interfaces are enabled and the status of every interface is shown as UP/UP.

Note

If you do not have an SFP+ transceiver for every port, verify the interfaces in stages. After checking the first set of interfaces, unplug the SFP+ transceivers and plug them in to the next set of ports. The SFP+ transceivers are not hot-swappable. Therefore, restart the MPX appliance after you connect the transceivers.

5. Run the following commands for each of the interfaces that are not in the UP/UP state:

- **enable interface 1/x**
- **enable interface 10/x**

where x is the new interface number.

6. Run the following command to verify that the status of the power supplies is normal: **stat system -detail**

Example

```
1 > stat system -detail
2 NetScaler Executive View
3 System Information:
4 Up since      Tue Dec  4 14:01:49 2018
5 Memory usage (MB)                859
6 InUse Memory (%)                 4.81
7 Number of CPUs                   5
8 System Health Statistics (Standard):
9 CPU 0 Core Voltage (Volts)       1.78
10 CPU 1 Core Voltage (Volts)      0.00
11 Main 3.3 V Supply Voltage       3.28
12 Standby 3.3 V Supply Voltage    3.28
13 +5.0 V Supply Voltage           4.90
14 +12.0 V Supply Voltage          11.81
15 Battery Voltage (Volts)         3.02
16 Intel CPU Vtt Power(Volts)      0.00
17 5V Standby Voltage(Volts)       5.05
18 Voltage Sensor2(Volts)          0.00
19 CPU Fan 0 Speed (RPM)           6900
20 CPU Fan 1 Speed (RPM)           6700
21 System Fan Speed (RPM)          6800
22 System Fan 1 Speed (RPM)        6800
23 System Fan 2 Speed (RPM)        6900
24 CPU 0 Temperature (Celsius)     44
25 CPU 1 Temperature (Celsius)     0
26 Internal Temperature (Celsius)  37
27 Power supply 1 status            NORMAL
28 Power supply 2 status            NORMAL
29 Power supply 3 status            NOT SUPPORTED
30 Power supply 4 status            NOT SUPPORTED
31 System Disk Statistics:
32 /flash Size (MB)                 16858
33 /flash Used (MB)                 323
34 /flash Available (MB)           15186
35 /flash Used (%)                  2
36 /var Size (MB)                  143802
```

```
37 /var Used (MB) 1880
38 /var Available (MB) 130418
39 /var Used (%) 1
40 System Health Statistics(Auxiliary):
41 Voltage 0 (Volts) 1.20
42 Voltage 1 (Volts) 1.20
43 Voltage 2 (Volts) 0.00
44 Voltage 3 (Volts) 0.00
45 Voltage 4 (Volts) 0.00
46 Voltage 5 (Volts) 0.00
47 Voltage 6 (Volts) 0.00
48 Voltage 7 (Volts) 0.00
49 Fan 0 Speed (RPM) 7000
50 Fan 1 Speed (RPM) 0
51 Fan 2 Speed (RPM) 0
52 Fan 3 Speed (RPM) 0
53 Temperature 0 (Celsius) 28
54 Temperature 1 (Celsius) 34
55 Temperature 2 (Celsius) 0
56 Temperature 3 (Celsius) 0
57 Done
58
59 <!--NeedCopy-->
```

7. Run the following command to generate a tar of system configuration data and statistics: **show techsupport**

Example

```
1 > show techsupport
2 showtechsupport data collector tool - $Revision: #13 $!
3 NetScaler version 11.1
4 Creating /var/tmp/support ....
5 The NS IP of this box is 10.221.44.30
6 This is not HA configuration
7 Copying selected configuration files ....
8 Running shell commands ....
9 Running CLI show commands ....
10 Collecting ns running configuration....
11 Collecting running gslb configuration....
12 Running CLI stat commands ....
13 Running vtysh commands ....
14 Copying newslog files ....
15 Copying core files from /var/core ....
16 Copying core files from /var/crash ....
```

```

17 Copying GSLB location database files ....
18 Copying GSLB auto sync log files ....
19 Copying Safenet Gateway log files ....
20 Copying messages, ns.log, dmesg and other log files ....
21 Creating archive ....
22 /var/tmp/support/support.tgz ----- points to ---> /var/tmp/support
    /collector_P_10.221.44.30_4Dec2018_14_14.tar.gz
23
24 Done
25
26 <!--NeedCopy-->

```

Note

The output of the command is available in the `/var/tmp/support/collector_<IP_address>_P_<date>.tar.gz` file. Copy this file to another computer for future reference. The output of the command might be helpful in case you want to contact Citrix Technical Support.

8. At the Citrix ADC command line interface, switch to the shell prompt. Type `shell`
9. Run the following command to verify that 270 MB of RAM is reserved for shared memory:


```
root@ns## dmesg | grep memory
```

Example

```

1 root@ns# dmesg | grep memory
2 real memory = 36507222016 (34816 MB)
3 avail memory = 32728735744 (31212 MB)
4 NS-KERN nsppe_rendezvous: NSPPE-02 on CPU3NS-KERN
    map_shared_mem_ioctl (cpu 2, NSPPE-01): Reserving 270 MB for
    shared memory type 0
5 root@ns#
6
7 <!--NeedCopy-->

```

10. Run the following command to verify that the appliance has 12 CPU cores: `root@ns## dmesg | grep cpu`

Example

```

1 root@ns# dmesg | grep cpu
2 cpu0 (BSP): APIC ID: 0
3 cpu1 (AP): APIC ID: 2
4 cpu2 (AP): APIC ID: 4
5 cpu3 (AP): APIC ID: 6
6 cpu4 (AP): APIC ID: 8

```

```

7  cpu5 (AP): APIC ID: 10
8  cpu6 (AP): APIC ID: 12
9  cpu7 (AP): APIC ID: 14
10 cpu0: <ACPI CPU> on acpi0
11 cpu1: <ACPI CPU> on acpi0
12 cpu2: <ACPI CPU> on acpi0
13 cpu3: <ACPI CPU> on acpi0
14 cpu4: <ACPI CPU> on acpi0
15 cpu5: <ACPI CPU> on acpi0
16 cpu6: <ACPI CPU> on acpi0
17 cpu7: <ACPI CPU> on acpi0
18 est0: <Enhanced SpeedStep Frequency Control> on cpu0
19 p4tcc0: <CPU Frequency Thermal Control> on cpu0
20 est1: <Enhanced SpeedStep Frequency Control> on cpu1
21 p4tcc1: <CPU Frequency Thermal Control> on cpu1
22 est2: <Enhanced SpeedStep Frequency Control> on cpu2
23 p4tcc2: <CPU Frequency Thermal Control> on cpu2
24 est3: <Enhanced SpeedStep Frequency Control> on cpu3
25 p4tcc3: <CPU Frequency Thermal Control> on cpu3
26 est4: <Enhanced SpeedStep Frequency Control> on cpu4
27 p4tcc4: <CPU Frequency Thermal Control> on cpu4
28 est5: <Enhanced SpeedStep Frequency Control> on cpu5
29 p4tcc5: <CPU Frequency Thermal Control> on cpu5
30 est6: <Enhanced SpeedStep Frequency Control> on cpu6
31 p4tcc6: <CPU Frequency Thermal Control> on cpu6
32 est7: <Enhanced SpeedStep Frequency Control> on cpu7
33 p4tcc7: <CPU Frequency Thermal Control> on cpu7
34 NS-KERN nsppe_rendezvous: NSPPE-02 on CPU3NS-KERN
    map_shared_mem_ioctl (cpu 2, NSPPE-01): Reserving 270 MB for
    shared memory type 0
35 root@ns#
36
37 <!--NeedCopy-->

```

11. Run the following command to verify that the /var drive is mounted as /dev/ad0s1e: root@ns
df -h

Example

```

1  root@ns# df -h
2  Filesystem      Size      Used    Avail Capacity  Mounted on
3  /dev/md0        354M      342M      5M      99%      /
4  devfs           1.0k      1.0k      0B      100%     /dev
5  procfs          4.0k      4.0k      0B      100%     /proc
6  /dev/ad0s1a     16G       323M     14G       2%       /flash

```



```
7 /dev/ad0s1e    140G    1.9G    127G    1%    /var
8 root@ns#
9
10 <!--NeedCopy-->
```

12. Run the `ns_hw_err.bash` script, which checks for latent hardware errors: `root@ns## /netscaler/ns_hw_err.bash`

Example

```
1 root@ns# ns_hw_err.bash
2 NetScaler NS11.1: Build 60.5.nc, Date: Oct  3 2018, 10:58:21
3 platform: serial JVFUJCZT1E
4 platform: sysid 30010 - NSMPX-8900 8*CPU+4*F1X+6*E1K+1*E1K+1*COL
   8955
5 HDD MODEL: ad0: 228936MB <MICRON M510DC MTFDDAK240MBP 0013> at
   ata0-master UDMA33
6
7 Generating the list of newnslog files to be processed...
8 Generating the events from newnslog files...
9 Checking for HDD errors...
10 Checking for HDD SMART errors...
11 Checking for Flash errors...
12     skipping flash check because HDD and flash are same physical
   device: ad0.
13     Please refer to HDD error output.
14 Checking for Mega Raid Controller errors...
15 Checking for SSL errors...
16 Checking for BIOS errors...
17 Checking for SMB errors...
18 Checking for MotherBoard errors...
19 Checking for CMOS errors...
20     License year: 2018: OK
21 License server failed at startup. Check /var/log/license.log
22 Vendor daemon failed at startup. Check /var/log/license.log
23 Checking for SFP/NIC errors...
24 Checking for Firmware errors...
25 Checking for License errors...
26 Checking for Undetected CPUs...
27 Checking for DIMM flaps...
28 Checking for LOM errors...
29 Checking the Power Supply Errors...
30 Checking for Hardware Clock errors...
31 *****
```

```
32 NS hardware check: Found 2 errors
33 *****
34 Script Done.
35 root@ns#
36 <!--NeedCopy-->
```

13. **Important:** Physically disconnect all ports except the LOM port, including the management port, from the network.
14. At the shell prompt, switch to the Citrix ADC command line. Type: **exit**
15. Run the following command to shut down the appliance: `shutdown -p now`

Example

```
1 > shutdown -p now
2 Are you sure you want to completely stop NetScaler (Y/N)? [N]:y
3 <!--NeedCopy-->
```


Upgrade the appliance

The upgrade process involves the following two steps:


- Replace the SSD
- Start the appliance

Replace the SSD

1. Locate the solid-state drive on the back panel of the appliance, as shown in the following figure:

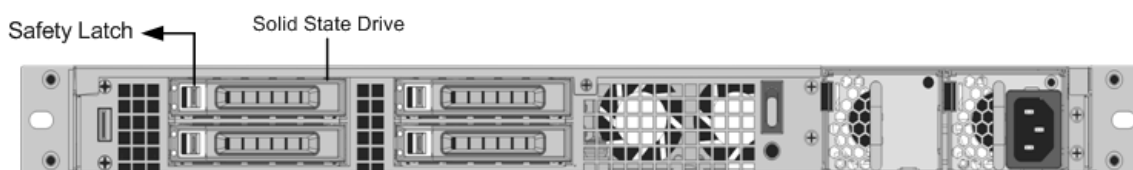

2. Verify that the replacement solid-state drive (SSD) is the one required for your Citrix ADC model. The Citrix label is on the top of the SSD. The SSD is pre-populated with a new version of the BIOS and a recent build of the required Service VM software.
3. Remove the currently installed SSD drive by pushing the safety latch of the drive cover to the right and pulling out the drive by its handle.
4. Open the drive handle on the new drive completely to the left, and insert the drive into the slot. The following figure shows the drive partially inserted. Push the drive all the way into the slot.

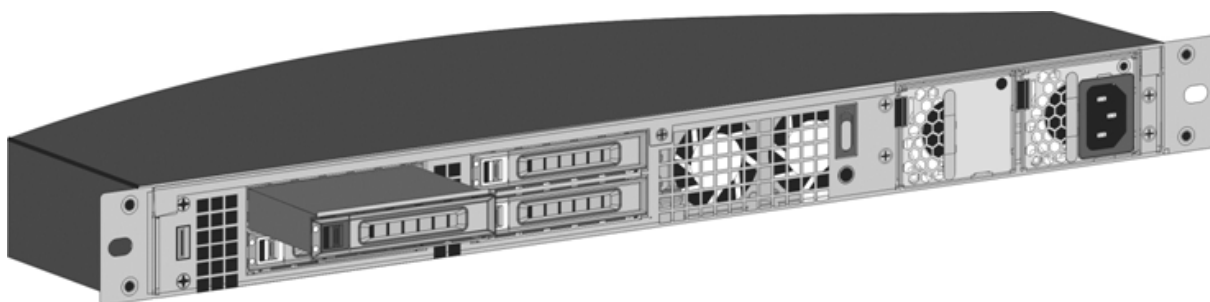

1. Close the handle flush with the rear side of the appliance so that the drive locks securely into the slot.

Important

The orientation of the solid-state drive is important. When you insert the drive, make sure that the Citrix product label is at the top.

Start the appliance

1. Start the Citrix ADC appliance. For instructions, see the Switching on the Appliance section in [Installing the hardware](#).

The conversion process takes approximately 30 minutes to complete. The conversion process performs the following actions:

- Updates the BIOS.
- Installs the Citrix Hypervisor and the Service VM operating system.
- Copies the Citrix ADC VPX image to the solid state drive for instance provisioning.

When the conversion begins, the LCD screen on the front bezel indicates NSMPX-8900, as shown in the following figure.

```
1 ![SDX 8900 before conversion](/en-us/citrix-hardware-platforms/sdx/
  media/89xx-before-conversion.png)
2
3 When the conversion is successful, the LCD indicates Citrix NSSDX -
  8900, as shown in the following figure.
4
5 ![SDX 8900 after conversion](/en-us/citrix-hardware-platforms/sdx/media
  /89xx-after-conversion.png)
6
7 > **Note**
8 >
9 > The serial number of the appliance remains the same.
```

1. Keep the console cable attached during the conversion process. Allow the process to complete, at which point the netscaler-sdx login: prompt appears.

2. When the appliance finishes the conversion process, it no longer has the previously working configuration. Therefore, you can access the appliance through a Web browser only. Use the default IP address: 192.168.100.1/16. Configure a computer on network 192.168.0.0 and connect it directly to the management port 0/1 of the appliance by using a cross-over Ethernet cable. Alternately, access the appliance through a network hub by using a straight-through Ethernet cable. Use the default credentials.
3. Select the **Configuration** tab.
4. Verify that the System Resource section displays CPU cores, SSL cores, and total memory for the Citrix ADC SDX appliance.
5. Select System node and click the Network Configuration link on the System page to modify the IP address of the Service VM.
6. In the Modify Network Configuration dialog box, specify the following details:
 - Interface—The interface through which clients connect to the Management Service. Possible values: 0/1, 0/2. Default: 0/1.
 - Citrix Hypervisor IP Address—The IP address of the Citrix Hypervisor.
 - Management Service IP Address—The IP address of the Management Service.
 - Netmask—The subnet mask for the subnet in which the SDX appliance is located.
 - Gateway—The default gateway for the network.
 - DNS Server—The IP address of the DNS server. *An optional parameter
7. Click **OK**.
8. Connect the Citrix ADC SDX appliance to a switch to access it through the network. Browse to the Management Service IP and log on with the default credentials.
9. For instructions for applying the licenses, see [Citrix ADC SDX Licensing Overview](#).

Convert a Citrix ADC MPX 15000 appliance to a Citrix ADC SDX 15000 appliance

December 9, 2020

You can convert a Citrix ADC MPX appliance to an ADC SDX appliance by upgrading the software through a new solid-state drive (SSD). Citrix supplies a field conversion kit to migrate a Citrix ADC MPX appliance to an SDX appliance.

The conversion requires all eight SSDs.

Note

Citrix recommends that you configure the lights out management (LOM) port of the appliance before starting the conversion process. For more information on the LOM port of the ADC appliance, see [Lights out management port of the Citrix ADC SDX appliance](#).

To convert an MPX appliance to an SDX appliance, you must access the appliance through a console cable attached to a computer or terminal. Before connecting the console cable, configure the computer or terminal to support the following configuration:

- VT100 terminal emulation
- 9600 baud
- 8 data bits
- 1 stop bit
- Parity and flow control set to NONE

Connect one end of the console cable to the RS232 serial port on the appliance, and the other end to the computer or terminal.

Note

To use a cable with an RJ-45 converter, insert the optional converter into the console port and attach the cable to it.

Citrix recommends you to connect a VGA monitor to the appliance to monitor the conversion process, because the LOM connection is lost during the conversion process.

With the cable attached, verify that the MPX appliance's components are functioning correctly. You are then ready to begin the conversion. The conversion process modifies the BIOS, installs a Citrix Hypervisor and a Service Virtual Machine image, and copies the ADC VPX image to the Solid State Drive.

The conversion process also sets up a redundant array of independent disks (RAID) controller for local storage and ADC VPX storage. SSD slots #1 and #2 are used for local storage and SSD slots #3 and #4 are used for ADC VPX storage.

After the conversion process, modify the appliance's configuration and apply a new license. You can then provision the VPX instances through the Management Service on what is now an ADC SDX appliance.

Verify proper operation of the MPX appliance's components

1. Access the console port and enter the administrator credentials.
2. Run the following command from the command line interface of the appliance to display the serial number: `show hardware`. You might need the serial number to log on to the appliance after the conversion.

Example

```
1 > show hardware
2 Platform: NSMPX-15000-50G 16*CPU+128GB+4*MLX(50)+8*F1X+2*E1K+2*2-
  CHIP COL 520400
3 Manufactured on: 9/13/2017
4 CPU: 2100MHZ
5 Host Id: 1862303878
6 Serial no: 4VCX9CUFN6
7 Encoded serial no: 4VCX9CUFN6
8 Netscaler UUID: d9de2de3-dc89-11e7-ab53-00e0ed5de5aa
9 BMC Revision: 5.56
10 Done
11 <!--NeedCopy-->
```

The serial number might be helpful when you want to contact Citrix Technical Support.

3. Run the following command to display the status of the active interfaces:

```
show interface
```

Example

```
1 > show interface
2
3 1) Interface 0/1 (Gig Ethernet 10/100/1000 Mbits) #4
4 flags=0xc020 <ENABLED, UP, UP, autoneg, HAMON, HEARTBEAT,
  802.1q>
5 MTU=1500, native vlan=1, MAC=0c:c4:7a:e5:3c:50, uptime 1
  h08m02s
6 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
7 throughput 0
8 Actual: media UTP, speed 1000, duplex FULL, fctl OFF,
  throughput 1000
9 LLDP Mode: NONE, LR Priority: 1024
10
11 RX: Pkts(19446) Bytes(1797757) Errs(0) Drops(19096) Stalls(0)
12 TX: Pkts(368) Bytes(75619) Errs(0) Drops(0) Stalls(0)
13 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
14 Bandwidth thresholds are not set.
15
16 2) Interface 0/2 (Gig Ethernet 10/100/1000 Mbits) #5
17 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
18 MTU=1500, native vlan=1, MAC=0c:c4:7a:e5:3c:51, downtime 1
  h08m15s
19 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
20 throughput 0
```

```
21 LLDP Mode: NONE, LR Priority: 1024
22
23 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
24 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
25 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
26 Bandwidth thresholds are not set.
27
28 3) Interface 10/1 (10G Ethernet) #6
29 flags=0x4000 <ENABLED, DOWN, down, autoneg, HAMON, HEARTBEAT,
30 802.1q>
31 MTU=1500, native vlan=200, MAC=00:e0:ed:5d:e5:76, downtime 1
32 h08m15s
33 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
34 throughput 0
35 LLDP Mode: NONE, LR Priority: 1024
36
37 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
38 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
39 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
40 Bandwidth thresholds are not set.
41 Rx Ring: Configured size=2048, Actual size=512, Type: Elastic
42
43 4) Interface 10/2 (10G Ethernet) #7
44 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
45 MTU=1500, native vlan=200, MAC=00:e0:ed:5d:e5:77, downtime 1
46 h08m15s
47 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
48 throughput 0
49 LLDP Mode: NONE, LR Priority: 1024
50
51 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
52 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
53 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
54 Bandwidth thresholds are not set.
55 Rx Ring: Configured size=2048, Actual size=512, Type: Elastic
56
57 5) Interface 10/3 (10G Ethernet) #8
58 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
59 MTU=1500, native vlan=1, MAC=00:e0:ed:5d:e5:78, downtime 1
60 h08m15s
61 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
62 throughput 0
63 LLDP Mode: NONE, LR Priority: 1024
64
65 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
```

```
62 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
63 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
64 Bandwidth thresholds are not set.
65 Rx Ring: Configured size=2048, Actual size=512, Type: Elastic
66
67 6) Interface 10/4 (10G Ethernet) #9
68 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
69 MTU=1500, native vlan=1, MAC=00:e0:ed:5d:e5:79, downtime 1
    h08m15s
70 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
71             throughput 0
72 LLDP Mode: NONE,                LR Priority: 1024
73
74 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
75 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
76 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
77 Bandwidth thresholds are not set.
78 Rx Ring: Configured size=2048, Actual size=512, Type: Elastic
79
80 7) Interface 10/5 (10G Ethernet) #0
81 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
82 MTU=1500, native vlan=1, MAC=00:e0:ed:5d:e5:aa, downtime 1
    h08m15s
83 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
84             throughput 0
85 LLDP Mode: NONE,                LR Priority: 1024
86
87 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
88 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
89 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
90 Bandwidth thresholds are not set.
91 Rx Ring: Configured size=2048, Actual size=512, Type: Elastic
92
93 8) Interface 10/6 (10G Ethernet) #1
94 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
95 MTU=1500, native vlan=1, MAC=00:e0:ed:5d:e5:ab, downtime 1
    h08m15s
96 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
97             throughput 0
98 LLDP Mode: NONE,                LR Priority: 1024
99
100 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
101 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
102 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
103 Bandwidth thresholds are not set.
```



```
104 Rx Ring: Configured size=2048, Actual size=512, Type: Elastic
105
106 9) Interface 10/7 (10G Ethernet) #2
107 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
108 MTU=1500, native vlan=1, MAC=00:e0:ed:5d:e5:ac, downtime 1
      h08m15s
109 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
110           throughput 0
111 LLDP Mode: NONE,           LR Priority: 1024
112
113 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
114 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
115 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
116 Bandwidth thresholds are not set.
117 Rx Ring: Configured size=2048, Actual size=512, Type: Elastic
118
119 10) Interface 10/8 (10G Ethernet) #3
120 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
121 MTU=1500, native vlan=1, MAC=00:e0:ed:5d:e5:ad, downtime 1
      h08m15s
122 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
123           throughput 0
124 LLDP Mode: NONE,           LR Priority: 1024
125
126 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
127 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
128 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
129 Bandwidth thresholds are not set.
130 Rx Ring: Configured size=2048, Actual size=512, Type: Elastic
131
132 11) Interface 50/1 (50G Ethernet) #13
133 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
134 MTU=1500, native vlan=1, MAC=24:8a:07:a3:1f:84, downtime 1
      h08m22s
135 Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
136           throughput 0
137 LLDP Mode: NONE,           LR Priority: 1024
138
139 RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
140 TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
141 NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
142 Bandwidth thresholds are not set.
143
144 12) Interface 50/2 (50G Ethernet) #12
145 flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
```

```
146     MTU=1500, native vlan=1, MAC=24:8a:07:a3:1f:6c, downtime 1
147         h08m22s
148     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
149         throughput 0
150     LLDP Mode: NONE,                LR Priority: 1024
151     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
152     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
153     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
154     Bandwidth thresholds are not set.
155
156 13) Interface 50/3 (50G Ethernet) #11
157     flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
158     MTU=1500, native vlan=1, MAC=24:8a:07:a3:1f:98, downtime 1
159         h08m22s
160     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
161         throughput 0
162     LLDP Mode: NONE,                LR Priority: 1024
163     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
164     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
165     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
166     Bandwidth thresholds are not set.
167
168 14) Interface 50/4 (50G Ethernet) #10
169     flags=0x4000 <ENABLED, DOWN, down, autoneg, HEARTBEAT, 802.1q>
170     MTU=1500, native vlan=1, MAC=24:8a:07:94:b9:b6, downtime 1
171         h08m22s
172     Requested: media AUTO, speed AUTO, duplex AUTO, fctl OFF,
173         throughput 0
174     LLDP Mode: NONE,                LR Priority: 1024
175     RX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
176     TX: Pkts(0) Bytes(0) Errs(0) Drops(0) Stalls(0)
177     NIC: InDisc(0) OutDisc(0) Fctls(0) Stalls(0) Hangs(0) Muted(0)
178     Bandwidth thresholds are not set.
179
180 15) Interface L0/1 (Netscaler Loopback interface) #14
181     flags=0x20008020 <ENABLED, UP, UP>
182     MTU=1500, native vlan=1, MAC=0c:c4:7a:e5:3c:50, uptime 1
183         h08m18s
184     LLDP Mode: NONE,                LR Priority: 1024
185     RX: Pkts(5073645) Bytes(848299459) Errs(0) Drops(0) Stalls(0)
186     TX: Pkts(9923625) Bytes(968741778) Errs(0) Drops(0) Stalls(0)
```

```
187     Bandwidth thresholds are not set.
188
189 Done
190 <!--NeedCopy-->
```

4. In the show interface command's output, verify that all the interfaces are enabled and the status of every interface is shown as UP/UP.

Notes:

>

>- The interface status is displayed as UP/UP only if the cables are connected to the interfaces.

>

>- If you do not have an SFP+ transceiver for every port, verify the interfaces in stages. After checking the first set of interfaces, unplug the SFP+ transceivers and plug them in to the next set of ports.

5. Run the following command for each of the interfaces that are not in the UP/UP state:

```
1 > enable interface 50/1
2 Done
3 > enable interface 50/2
4 Done
5 > enable interface 50/3
6 Done
7 > enable interface 50/4
8 Done
9 <!--NeedCopy-->
```

Where x is the new interface number

6. Run the following command to verify that the status of the power supplies is normal:

```
stat system -detail
```

Example

```
1 > stat system -detail
2
3 Citrix ADC Executive View
4
5 System Information:
6 Up since          Sat Dec  5 04:17:29 2020
7 Up since(Local)  Sat Dec  5 04:17:29 2020
8 Memory usage (MB)                4836
9 InUse Memory (%)                  4.08
```

10	Number of CPUs	13
11		
12	System Health Statistics (Standard):	
13	CPU 0 Core Voltage (Volts)	1.80
14	CPU 1 Core Voltage (Volts)	1.80
15	Main 3.3 V Supply Voltage	3.35
16	Standby 3.3 V Supply Voltage	3.23
17	+5.0 V Supply Voltage	5.00
18	+12.0 V Supply Voltage	12.06
19	Battery Voltage (Volts)	3.02
20	Intel CPU Vtt Power(Volts)	0.00
21	5V Standby Voltage(Volts)	4.95
22	Voltage Sensor2(Volts)	0.00
23	CPU Fan 0 Speed (RPM)	3500
24	CPU Fan 1 Speed (RPM)	3600
25	System Fan Speed (RPM)	3600
26	System Fan 1 Speed (RPM)	3600
27	System Fan 2 Speed (RPM)	3500
28	CPU 0 Temperature (Celsius)	37
29	CPU 1 Temperature (Celsius)	47
30	Internal Temperature (Celsius)	26
31	Power supply 1 status	NORMAL
32	Power supply 2 status	NORMAL
33	Power supply 3 status	NOT SUPPORTED
34	Power supply 4 status	NOT SUPPORTED
35		
36	System Disk Statistics:	
37	/flash Size (MB)	23801
38	/flash Used (MB)	7009
39	/flash Available (MB)	14887
40	/flash Used (%)	32
41	/var Size (MB)	341167
42	/var Used (MB)	56502
43	/var Available (MB)	257371
44	/var Used (%)	18
45		
46	System Health Statistics(Auxiliary):	
47	Voltage 0 (Volts)	1.20
48	Voltage 1 (Volts)	1.20
49	Voltage 2 (Volts)	1.20
50	Voltage 3 (Volts)	1.20
51	Voltage 4 (Volts)	1.54
52	Voltage 5 (Volts)	0.00
53	Voltage 6 (Volts)	0.00
54	Voltage 7 (Volts)	0.00

```
55 Fan 0 Speed (RPM) 3600
56 Fan 1 Speed (RPM) 0
57 Fan 2 Speed (RPM) 0
58 Fan 3 Speed (RPM) 0
59 Temperature 0 (Celsius) 24
60 Temperature 1 (Celsius) 30
61 Temperature 2 (Celsius) 0
62 Temperature 3 (Celsius) 0
63 Done
64 <!--NeedCopy-->
```

7. Run the following command to generate a tar of system configuration data and statistics:

```
show techsupport
```

Example

```
1 > show techsupport
2
3 showtechsupport data collector tool - $Revision$!
4 NetScaler version 13.0
5 The NS IP of this box is 10.217.206.43
6 This is not HA configuration
7 Copying selected configuration files ....
8 Running shell commands ....
9 Running CLI show commands ....
10 Collecting ns running configuration....
11 Collecting running gslb configuration....
12 Running CLI stat commands ....
13 Running vtysh commands ....
14 Copying newslog files ....
15 Copying core files from /var/core ....
16 Copying core files from /var/crash ....
17 Copying GSLB location database files ....
18 Copying GSLB auto sync log files ....
19 Copying Safenet Gateway log files ....
20 Copying messages, ns.log, dmesg and other log files ....
21 Creating archive ....
22 /var/tmp/support/support.tgz ---- points to ---> /var/tmp/support
    /collector_P_10.217.206.43_5Dec2020_05_32.tar.gz
23
24 showtechsupport script took 1 minute(s) and 17 second(s) to
    execute.
25 Done
26 <!--NeedCopy-->
```

Note

The output of the command is available in the `/var/tmp/support/collector_<IP_address>_P_<date>.tar.gz` file. Copy this file to another computer for future reference. The output of the command might be helpful when you want to contact Citrix Technical Support.

8. At the command line interface, switch to the shell prompt. Type: `shell`

Example

```
1 > shell
2 Copyright (c) 1992-2013 The FreeBSD Project.
3 Copyright (c) 1979, 1980, 1983, 1986, 1988, 1989, 1991, 1992,
   1993, 1994
4   The Regents of the University of California. All rights
   reserved.
5
6 root@ns#
7 <!--NeedCopy-->
```

9. Run the following command to verify the number of Cavium cards available depending upon your appliance:

```
root@ns## grep "memory"/var/nslog/dmesg.boot
```

Example

```
1 root@ns# grep "memory" /var/nslog/dmesg.boot
2 real memory = 139586437120 (133120 MB)
3 avail memory = 132710871040 (126562 MB)
4 root@ns#
5 <!--NeedCopy-->
```

10. Run the following command to verify the number of CPU cores depending upon your appliance:

```
root@ns## grep "cpu"/var/nslog/dmesg.boot
```

Example

```
1 root@ns# grep "cpu" /var/nslog/dmesg.boot
2 cpu0 (BSP): APIC ID: 0
3 cpu1 (AP): APIC ID: 2
4 cpu2 (AP): APIC ID: 4
5 cpu3 (AP): APIC ID: 6
6 cpu4 (AP): APIC ID: 8
7 cpu5 (AP): APIC ID: 10
8 cpu6 (AP): APIC ID: 12
9 cpu7 (AP): APIC ID: 14
```

```
10 cpu8 (AP): APIC ID: 16
11 cpu9 (AP): APIC ID: 18
12 cpu10 (AP): APIC ID: 20
13 cpu11 (AP): APIC ID: 22
14 cpu12 (AP): APIC ID: 24
15 cpu13 (AP): APIC ID: 26
16 cpu14 (AP): APIC ID: 28
17 cpu15 (AP): APIC ID: 30
18 cpu0: <ACPI CPU> on acpi0
19 cpu1: <ACPI CPU> on acpi0
20 cpu2: <ACPI CPU> on acpi0
21 cpu3: <ACPI CPU> on acpi0
22 cpu4: <ACPI CPU> on acpi0
23 cpu5: <ACPI CPU> on acpi0
24 cpu6: <ACPI CPU> on acpi0
25 cpu7: <ACPI CPU> on acpi0
26 cpu8: <ACPI CPU> on acpi0
27 cpu9: <ACPI CPU> on acpi0
28 cpu10: <ACPI CPU> on acpi0
29 cpu11: <ACPI CPU> on acpi0
30 cpu12: <ACPI CPU> on acpi0
31 cpu13: <ACPI CPU> on acpi0
32 cpu14: <ACPI CPU> on acpi0
33 cpu15: <ACPI CPU> on acpi0
34 est0: <Enhanced SpeedStep Frequency Control> on cpu0
35 p4tcc0: <CPU Frequency Thermal Control> on cpu0
36 est1: <Enhanced SpeedStep Frequency Control> on cpu1
37 p4tcc1: <CPU Frequency Thermal Control> on cpu1
38 est2: <Enhanced SpeedStep Frequency Control> on cpu2
39 p4tcc2: <CPU Frequency Thermal Control> on cpu2
40 est3: <Enhanced SpeedStep Frequency Control> on cpu3
41 p4tcc3: <CPU Frequency Thermal Control> on cpu3
42 est4: <Enhanced SpeedStep Frequency Control> on cpu4
43 p4tcc4: <CPU Frequency Thermal Control> on cpu4
44 est5: <Enhanced SpeedStep Frequency Control> on cpu5
45 p4tcc5: <CPU Frequency Thermal Control> on cpu5
46 est6: <Enhanced SpeedStep Frequency Control> on cpu6
47 p4tcc6: <CPU Frequency Thermal Control> on cpu6
48 est7: <Enhanced SpeedStep Frequency Control> on cpu7
49 p4tcc7: <CPU Frequency Thermal Control> on cpu7
50 est8: <Enhanced SpeedStep Frequency Control> on cpu8
51 p4tcc8: <CPU Frequency Thermal Control> on cpu8
52 est9: <Enhanced SpeedStep Frequency Control> on cpu9
53 p4tcc9: <CPU Frequency Thermal Control> on cpu9
54 est10: <Enhanced SpeedStep Frequency Control> on cpu10
```

```

55 p4tcc10: <CPU Frequency Thermal Control> on cpu10
56 est11: <Enhanced SpeedStep Frequency Control> on cpu11
57 p4tcc11: <CPU Frequency Thermal Control> on cpu11
58 est12: <Enhanced SpeedStep Frequency Control> on cpu12
59 p4tcc12: <CPU Frequency Thermal Control> on cpu12
60 est13: <Enhanced SpeedStep Frequency Control> on cpu13
61 p4tcc13: <CPU Frequency Thermal Control> on cpu13
62 est14: <Enhanced SpeedStep Frequency Control> on cpu14
63 p4tcc14: <CPU Frequency Thermal Control> on cpu14
64 est15: <Enhanced SpeedStep Frequency Control> on cpu15
65 p4tcc15: <CPU Frequency Thermal Control> on cpu15
66 root@ns#
67 <!--NeedCopy-->

```

11. Run the following command to verify that the /var drive is mounted as /dev/ ar0s1a:
 root@ns## df -h

Example

```

1 root@ns# df -h
2 Filesystem      Size      Used    Avail Capacity  Mounted on
3 /dev/md0        422M      404M     9.1M    98%      /
4 devfs           1.0k      1.0k      0B     100%     /dev
5 procfs          4.0k      4.0k      0B     100%     /proc
6 /dev/ar0s1a     23G       6.9G     14G     32%     /flash
7 /dev/ar0s1e    333G       32G     274G     10%     /var
8 root@ns#
9 <!--NeedCopy-->

```

12. Type the following command to run the ns_hw_err.bash script, which checks for latent hardware errors: root@ns

```
## ns_hw_err.bash
```

Example

```

1 root@ns# ns_hw_err.bash
2 NetScaler NS13.0: Build 71.3602.nc, Date: Nov 12 2020, 07:26:41
   (64-bit)
3 platform: serial 4VCX9CUFN6
4 platform: sysid 520400 - NSMPX-15000-50G 16*CPU+128GB+4*MLX(50)+8*
   F1X+2*E1K+2*2-CHIP COL 8955
5 HDD MODEL: ar0: 434992MB <Intel MatrixRAID RAID1> status: READY
6
7 Generating the list of newnslog files to be processed...
8 Generating the events from newnslog files...

```



```
 9 Checking for HDD errors...
10 Checking for HDD SMART errors...
11 Checking for Flash errors...
12 Checking for Mega Raid Controller errors...
13 Checking for SSL errors...
14 Dec  5 06:00:31 <daemon.err> ns monit[996]: 'safenet_gw' process
    is not running
15 Checking for BIOS errors...
16 Checking for SMB errors...
17 Checking for MotherBoard errors...
18 Checking for CMOS errors...
19 License year: 2020: OK
20 Checking for SFP/NIC errors...
21 Dec  5 06:02:32 <daemon.err> ns monit[996]: 'safenet_gw' process
    is not running
22 Checking for Firmware errors...
23 Checking for License errors...
24 Checking for Undetected CPUs...
25 Checking for DIMM flaps...
26 Checking for Memory Channel errors...
27 Checking for LOM errors...
28 Checking the Power Supply Errors...
29 Checking for Hardware Clock errors...
30 Script Done.
31 root@ns#
32 <!--NeedCopy-->
```

13. **Important:** Physically disconnect all ports except the LOM port, including the management port, from the network.
14. At the shell prompt, switch to the ADC command line. Type: `exit`

Example

```
1 root@ns# exit
2 logout
3 Done
4 <!--NeedCopy-->
```

15. Run the following command to shut down the appliance. You are asked if you want to completely stop the ADC. Type: `shutdown -p now`

Example

```
1 > shutdown -p now
2 Are you sure you want to completely stop NetScaler (Y/N)? [N]:y
```


```
3 Done
4 > Dec 5 06:09:11 <auth.notice> ns shutdown: power-down by root:
5 Dec 5 06:09:13 <auth.emerg> ns init: Rebooting via init mechanism
6 Dec 5 06:09:13 <syslog.err> ns syslogd: exiting on signal 15
7 Dec 5 06:09:13 aslearn[1662]: before pthread_join(), task name:
  Aslearn_Packet_Loop_Task
8 Dec 5 06:09:15 aslearn[1662]: Exiting function ns_do_logging
9 Dec 5 06:09:15 aslearn[1662]: before pthread_join(), task name:
  Aslearn_WAL_Cleanup_Task
10 Dec 5 06:09:15 aslearn[1662]: before pthread_join(), task name:
  Aslearn_HA_Primary_Task
11 Dec 5 06:09:15 aslearn[1662]: 1662 exiting gracefully
12 Dec 5 06:09:18 [1672]: nsmnet_tcpipconnect: connect() failed;
  returned -1 errno=61
13 qat0: qat_dev0 stopped 12 acceleration engines
14 pci4: Resetting device
15 qat1: qat_dev1 stopped 12 acceleration engines
16 pci6: Resetting device
17 qat2: qat_dev2 stopped 12 acceleration engines
18 pci132: Resetting device
19 qat3: qat_dev3 stopped 12 acceleration engines
20 pci134: Resetting device
21 Dec 5 06:09:33 init: some processes would not die; ps axl advised
22 reboot initiated by init with parent kernel
23 Waiting (max 60 seconds) for system process `vnlru' to stop...done
24 Waiting (max 60 seconds) for system process `bufdaemon' to stop...
  done
25 Waiting (max 60 seconds) for system process `syncer' to stop...
26 Syncing disks, vnodes remaining...0 0 0 done
27 All buffers synced.
28 Uptime: 1h53m18s
29 ixl_shutdown: lldp start 0
30 ixl_shutdown: lldp start 0
31 ixl_shutdown: lldp start 0
32 ixl_shutdown: lldp start 0
33 usb0: Controller shutdown
34 uhub0: at usb0, port 1, addr 1 (disconnected)
35 usb0: Controller shutdown complete
36 usb1: Controller shutdown
37 uhub1: at usb1, port 1, addr 1 (disconnected)
38 ugen1.2: <vendor 0x8087> at usb1 (disconnected)
39 uhub3: at uhub1, port 1, addr 2 (disconnected)
40 ugen1.3: <FTDI> at usb1 (disconnected)
41 uftdi0: at uhub3, port 1, addr 3 (disconnected)
42 ugen1.4: <vendor 0x1005> at usb1 (disconnected)
```

```
43 umass0: at uhub3, port 3, addr 4 (disconnected)
44 (da0:umass-sim0:0:0:0): lost device - 0 outstanding, 0 refs
45 (da0:umass-sim0:0:0:0): removing device entry
46 usb1: Controller shutdown complete
47 usb2: Controller shutdown
48 uhub2: at usb2, port 1, addr 1 (disconnected)
49 ugen2.2: <vendor 0x8087> at usb2 (disconnected)
50 uhub4: at uhub2, port 1, addr 2 (disconnected)
51 ugen2.3: <vendor 0x0557> at usb2 (disconnected)
52 uhub5: at uhub4, port 7, addr 3 (disconnected)
53 ugen2.4: <vendor 0x0557> at usb2 (disconnected)
54 ukbd0: at uhub5, port 1, addr 4 (disconnected)
55 ums0: at uhub5, port 1, addr 4 (disconnected)
56 usb2: Controller shutdown complete
57 ixl_shutdown: lldp start 0
58 ixl_shutdown: lldp start 0
59 ixl_shutdown: lldp start 0
60 ixl_shutdown: lldp start 0
61 acpi0: Powering system off
62 <!--NeedCopy-->
```

Upgrade the appliance

To upgrade the appliance, follow these steps:

1. Power off the ADC appliance.
2. Locate two solid-state drives (SSDs) on the back of the appliance in slot #1 and slot #2, as shown in the following figure:

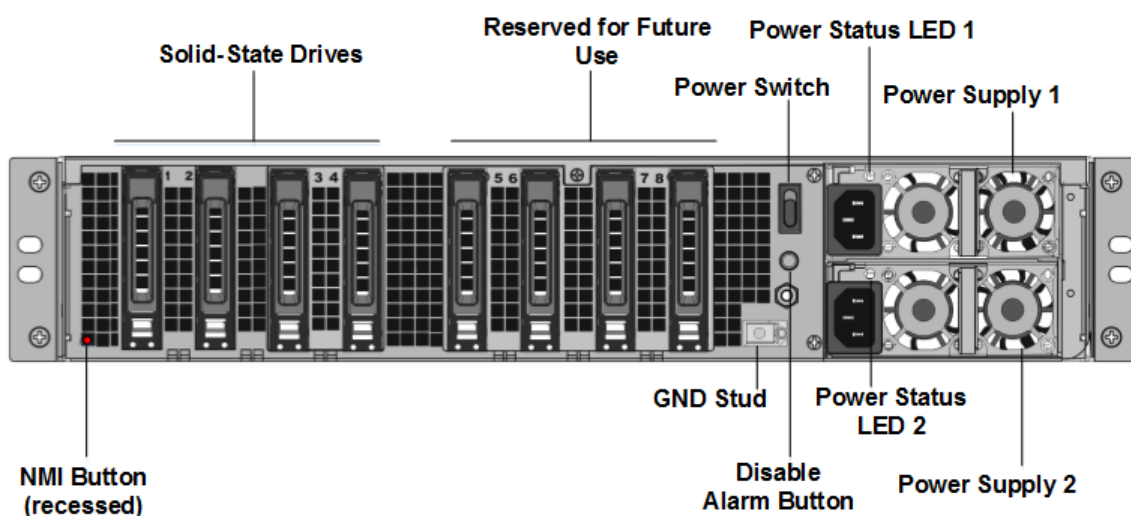

3. Verify that the replacement solid-state drives (SSDs) are the ones required for your ADC model. The conversion requires minimum of four SSDs. The Citrix label is on the top of one of the SSDs. The SSD is pre-populated with a new version of the BIOS and a recent build of the required ADC SDX Management Service. This SSD must be installed in slot # 1.
4. Remove the SSDs by pushing the safety latch of the drive cover down while pulling the drive handle.
5. On the new Citrix Certified SSD drive, open the drive handle completely to the left. Then insert the new drive into the slot #1 as far as possible.
6. To seat the drive, close the handle flush with the rear side of the appliance so that the drive locks securely into the slot.

Important: The orientation of the SSD is important. When you insert the drive, make sure that the Citrix product label is at the side.

7. Insert a second Citrix certified SSD, which matches the capacity of the SSD in slot #1, in slot # 2.

Note: If the license of your appliance is 14040 40G, 14060 40G, 14080 40G, insert more blank Citrix certified SSDs in slots #3, #4, #5, and #6.

ADC SDX Model	Included Virtual Instances	Platform Maximum	SSDs included on base model	Extra SSDs for max instances
SDX 15020/SDX 15020-50G	5	55	Two 240 GB RAID-supported removable boot solid-state drives (SSDs), (slots 1 and 2). Two 240 GB RAID-supported removable storage repositories (slots 3 and 4 paired) SSDs, and four 480 GB storage repositories (slots 5–6 paired and 7–8 paired) SSDs.	NA

SDX 15030/SDX 15030-50G	20	55	Two 240 GB RAID-supported removable boot solid-state drives (SSDs), (slots 1 and 2). Two 240 GB RAID-supported removable storage repositories (slots 3 and 4 paired) SSDs, and four 480 GB storage repositories (slots 5–6 paired and 7–8 paired) SSDs.	NA
----------------------------	----	----	---	----

Important

Mixing and matching of old and new SSDs is not supported. SSDs in slot #1 and slot #2, which constitute the first RAID pair (local storage), must be of the same size and type. Similarly, SSDs in slot #3 and slot #4, which constitute the second RAID pair (VPX storage), must be of the same size and type. Use only drives that are part of the provided conversion kit.

8. Disconnect all network cables from the data ports and the management ports.
9. Start the ADC appliance. For instructions, see “Switching on the Appliance” in Installing the Hardware.

The conversion process can run for approximately 30 minutes, during which you must not power cycle the appliance. The entire conversion process might not be visible on the console and might appear to be unresponsive.

The conversion process updates the BIOS, installs the Citrix Hypervisor and the Management Service Operating system. It also copies the ADC VPX image to the SSD for instance provisioning, and forms the Raid1 pair.

Note: The serial number of the appliance remains the same.

10. Keep the console cable attached during the conversion process. Allow the process to complete, at which point the SDX login: prompt appears.
11. During the conversion process the LOM port connection might be lost as it resets the IP address to the default value of 192.168.1.3. The conversion status output is available on the VGA monitor.
12. The default credentials for the Citrix Hypervisor are changed to root/nsroot after the appliance is converted from an MPX to SDX. If this password does not work, try typing nsroot/the serial number of the appliance. The serial number bar code is available at the back of the appliance, and is also available in the output of the `show hardware` command.
13. To make sure that the conversion is successful, verify that the FVT result indicates success. Run the following command: `tail /var/log/fvt/fvt.log`

Reconfigure the converted appliance

After the conversion process, the appliance no longer has its previous working configuration. Therefore, you can access the appliance through a web browser only by using the default IP address: 192.168.100.1/16. Configure a computer on network 192.168.0.0 and connect it directly to the appliance's management port (0/1) with a cross-over Ethernet cable. Alternately, access the ADC SDX appliance through a network hub by using a straight through Ethernet cable. Use the default credentials to log on, and then do the following:

1. Select the Configuration tab.
2. Verify that the System Resource section displays the accurate number of CPU cores, SSL cores, and the total memory for your ADC SDX appliance.
3. Select the **System** node and, under **Set Up Appliance**, click **Network Configuration** to modify the network information of the Management Service.
4. In the **Modify Network Configuration** dialog box, specify the following details:
 - Interface*—The interface through which clients connect to the Management Service. Possible values: 0/1, 0/2. Default: 0/1.
 - Citrix Hypervisor IP Address*—The IP address of Citrix Hypervisor.
 - Management Service IP Address*—The IP address of the Management Service.
 - Netmask*—The subnet mask for the subnet in which the SDX appliance is located.
 - Gateway*—The default gateway for the network.
 - DNS Server—The IP address of the DNS server.

*A mandatory parameter

5. Click **OK**. Connection to the Management Service is lost as the network information was changed.

6. Connect the ADC SDX appliance's management port 0/1 to a switch to access it through the network. Browse to the IP address used earlier and log on with the default credentials.
7. Apply the new licenses. For instructions, see [SDX Licensing Overview](#).
8. Navigate to **Configuration > System** and, in the **System Administration** group, click **Reboot Appliance**. Click **Yes** to confirm. You are now ready to provision the VPX instances on the ADC SDX appliance. For instructions, see [Provisioning Citrix ADC instances](#).

Troubleshooting

February 11, 2019

Following is the list of troubleshooting articles for Citrix ADC SDX hardware issues:

1. Troubleshooting Citrix ADC Power Supply Issues: <https://support.citrix.com/article/CTX202340>
2. Troubleshooting Citrix ADC Small Form Pluggable (SFP) Issues: <https://support.citrix.com/article/CTX236074>
3. Troubleshooting Citrix ADC SSL Card Issues: <https://support.citrix.com/article/CTX236094>

**Locations**

Corporate Headquarters | 851 Cypress Creek Road Fort Lauderdale, FL 33309, United States
Silicon Valley | 4988 Great America Parkway Santa Clara, CA 95054, United States

© 2021 Citrix Systems, Inc. All rights reserved. Citrix, the Citrix logo, and other marks appearing herein are property of Citrix Systems, Inc. and/or one or more of its subsidiaries, and may be registered with the U.S. Patent and Trademark Office and in other countries. All other marks are the property of their respective owner(s).